



User's Guide

Shop online at

omega.com®

Ω OMEGA®

omega.com

e-mail: info@omega.com

*For latest product manuals:
omegamanual.info*

ISO 9001
CERTIFIED
CORPORATE QUALITY
STAMFORD, CT

ISO 9002
CERTIFIED
CORPORATE QUALITY
MANCHESTER, UK



**DPG9031
DPG9131
DPG9231
DPG9046
DPG9146
DPG9246
DPG9045
DPG9145
DPG9245
DPG9030
DPG9130
DPG9230**



Digital Industrial Gauge



OMEGAnet® Online Service www.omega.com	Internet e-mail info@omega.com
---	---

Servicing North America:

USA: One Omega Drive, Box 4047
ISO 9001 Certified Stamford CT 06907-0047
Tel: (203) 359-1660 FAX: (203) 359-7700
e-mail: info@omega.com

Canada: 976 Bergar
Laval (Quebec) H7L 5A1, Canada
Tel: (514) 856-6928 FAX: (514) 856-6886
e-mail: info@omega.ca

For immediate technical or application assistance:

USA and Canada: Sales Service: 1-800-826-6342 / 1-800-TC-OMEGA®
Customer Service: 1-800-622-2378 / 1-800-622-BEST®
Engineering Service: 1-800-872-9436 / 1-800-USA-WHEN®
TELEX: 996404 EASYLINK: 62968934 CABLE: OMEGA

Mexico: En Español: (001) 203-359-7803 e-mail: espanol@omega.com
FAX: (001) 203-359-7807 info@omega.com.mx

Servicing Europe:

Benelux: Postbus 8034, 1180 LA Amstelveen, The Netherlands
Tel: +31 (0)20 3472121 FAX: +31 (0)20 6434643
Toll Free in Benelux: 0800 0993344
e-mail: sales@omegaeng.nl

Czech Republic: Frystatska 184, 733 01 Karvina, Czech Republic
Tel: +420 (0)59 6311899 FAX: +420 (0)59 6311114
Toll Free: 0800-1-66342 e-mail: info@omegashop.cz

France: 11, rue Jacques Cartier, 78280 Guyancourt, France
Tel: +33 (0)1 61 37 2900 FAX: +33 (0)1 30 57 5427
Toll Free in France: 0800 466 342
e-mail: sales@omega.fr

Germany/Austria: Daimlerstrasse 26, D-75392 Deckenpfronn, Germany
Tel: +49 (0)7056 9398-0 FAX: +49 (0)7056 9398-29
Toll Free in Germany: 0800 639 7678
e-mail: info@omega.de

United Kingdom: One Omega Drive, River Bend Technology Centre
ISO 9002 Certified Northbank, Irlam, Manchester
M44 5BD United Kingdom
Tel: +44 (0)161 777 6611 FAX: +44 (0)161 777 6622
Toll Free in United Kingdom: 0800-488-488
e-mail: sales@omega.co.uk

It is the policy of OMEGA to comply with all worldwide safety and EMC/EMI regulations that apply. OMEGA is constantly pursuing certification of its products to the European New Approach Directives. OMEGA will add the CE mark to every appropriate device upon certification.

The information contained in this document is believed to be correct, but OMEGA Engineering, Inc. accepts no liability for any errors it contains, and reserves the right to alter specifications without notice.

WARNING: These products are not designed for use in, and should not be used for, human applications.

Congratulations on your purchase of the Omega® digital industrial gauge. This feature-packed gauge offers a menu-driven display for easy customization. User selectable features include 12 units of measurement, password protected calibration and disable functions, adjustable bar graph and update rate. A five digit display for maximum resolution is standard. Optional 4-20mA output, switching and line- power add to the versatility of the gauge. With the range printed on the keypad, Omega digital gauges meet ASME B40.7 specification. See a complete listing of product features and specifications on pages 18.

TABLE OF CONTENTS

Quick Reference	6-7
Keypad Functions	8-9
• ON/OFF KEY • ZERO/CLEAR KEY • MIN/MAX KEY ▼ (down arrow key) • MENU KEY • BACKLITE KEY ▲ (up arrow key) • ENTER KEY	
MENU Functions (MENU Mode)	10-17
• Engineering Units • CONFIG Mode • Set Password • Recalibration of Gauge • Zero Key Adjustment • Disabling Menu Options • Bar Graph Options • Auto Off Options • Update Options for Displayed Pressure • Dampening Options • Backlite Options (Backlite Optional) • Set Switch(es) Option(s) (Switches Optional)	
Specifications	18
Ranges	19
Display Messages	19
Wiring Diagrams	20-30
Gauge Installation & Maintenance	32-34
• Mounting • Battery Replacement & Installation	

QUICK RE

*.88" high digital display (4½" case)
.60 high digital display(3" case)*

*Bar graph
% of full scale*

*Flashing display when unit
pressured below zero*

*Press to indicate minimum
or maximum pressure
gauge has measured
Press again to return to
pressure units*

Press to read menu



*UNITS (Pressure)
ENGLISH
INHG
PSI*
INH2O
@ 4°C, 20°C, 60°F
FTW
FTSW
METRIC
BAR
MBAR
KPA
CMH2O
KG/CM2*

*UPDATE RATE
(Pressure measurement
per second)
10x (100 MS)*
5x (200 MS)
2x (500 MS)
1x (1 Sec)*

*BACKLITE
(Off options)
Never
2 SEC
5 SEC*
15 MIN
30 MIN*



REFERENCE

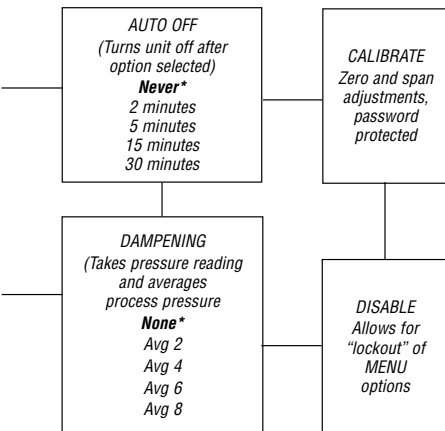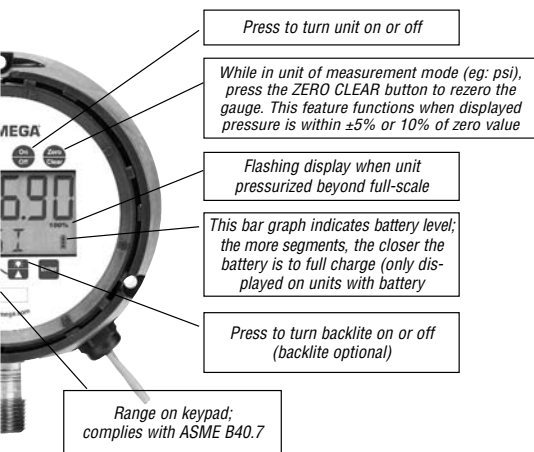

**Indicates Default*

KEYPAD FUNCTIONS



Turns the gauge on and off. When pressing the ON/OFF key while in the off position, gauge start-up display first indicates the software version followed by the model number and gauge pressure range. The gauge will then display indicated pressure and be ready for use.



Press this key for one second prior to gauge usage to rezero any initial zero shift. If zero shift is greater than programmed zero allowance, the gauge will display OFFSET (blinking) for 1 second, then return to the measure mode. To clear minimum and maximum values, press ZERO/CLR button (when min/max values are indicated). Gauge will auto advance once zeroed.



The Max/Min key allows review of minimum and maximum pressure values since unit start-up or last push of the clear key. Press key to:

- 1) Indicate maximum pressure.
- 2) Indicate minimum pressure.
- 3) Exit MAX/MIN mode and return the unit to pressure measurement mode. To clear minimum and maximum values press ZERO/CLR key (must be in MAX/MIN mode).

The ▼ (down arrow key) is used in the MENU mode, see following MENU key section.

KEYPAD FUNCTIONS



This key allows for customization of the gauge. Pressing the MENU key allows cycling through the main MENU items; UNITS, CONFIG, GRAPH, OFF, UPDAT & DAMP. Any item changed in the Menu become the new default setting(s). Revised settings are saved in the event of power loss.

The ▲ (up arrow key) or ▼ (down arrow key) on the keypad allows for scrolling through the MENU options to increase or decrease numeric values as required. If in the menu mode, gauge will automatically advance to measure mode once selected MENU item has been set.



Key for gauge
with Backlite

Key for gauge
without Backlite
displayed with
▲ (up arrow
icon only)

This key manually turns the backlight on or off. five options are available. They include NEVER, 10 sec, 30, sec, 1 min, 5 min*. With the NEVER option, the gauge BACKLITE will remain lit whenever the gauge is in the ON mode or until the BACKLITE button is pushed again. Options, 10 sec, 30 sec, 1 min, 5 min*. allow the BACK-LITE to automatically turn-off after a selected period of time.

To use the BACKLITE option:

Step 1: Press the MENU key.

Step 2: Press the ▲ (up arrow key) or ▼ (down arrow key) until the word LITE appears.

Step 3: Press ENTER.

Step 4: Press the ▲ (up arrow key) or ▼ (down arrow key) to select the BACKLITE option.

Step 5: Press the ENTER key to finalize your choice of LITE options.

KEYPAD FUNCTIONS



This key allows for selecting gauge features in the menu finalizing selection. Use of the enter key is described throughout operating instructions.

MENU OPTIONS

UNITS: 12 units of measurement are available: psi, mmHG, inH₂O with three temperature options: 20°C, 60°F, 4°C*, mBar, inHg, ftH₂O, mPa, kPa, kg/cm² and bar.

Step 1: Press the MENU key until the word UNITS appears.

Step 2: Press Enter.

Step 3: Press the ▲ (up arrow key) or ▼ (down arrow key) to select the required unit of measure.

Step 4: Press ENTER to finalize the UNIT selection.

Note: For inH₂O range with three temperature options, press the ▲ (up arrow key) and ▼ (down arrow key) to select the desired temperature, then press ENTER to finalize the UNIT selection.

CONFIG: This option allows access to additional Menu options. Options include:

- **ENTPW** or enter password (*this appears as a sub-menu in the CONFIG mode if a user password has been set*).
- **RECAL** (allows for zero, span and mid-scale calibration of the gauge).
- **ObUTN** or zero key (allows for adjustment of % of range that can be zeroed),
- **dISAb**, allows for disabling MENU options.
- **SETPW:** This feature allows for a user defined numeric password. If a user password is not set, all features in the CONFIG mode will be accessible without a password. If a user password is set, all items in the CONFIG menu options are accessible with or without a user password. If a user password is programmed, it will be required to access the CONFIG menu options.

*Indicates default.

KEYPAD FUNCTIONS

MENU FUNCTIONS

How to Use Your Menu Functions

To set a user password (SETPW):

Step 1: Press the Menu key on the keypad

Step 2: Press the ▲ (up arrow key) or ▼ (down arrow key) until the word CONFIG appears.

Step 3: Press Enter. The word SETPW appears on the gauge display

Step 4: Press Enter. A five digit numeric password is now required.

Step 5: Press the ▲ (up arrow key) or ▼ (down arrow key) on the keypad to select the first digit of the password.

Step 6: Press ENTER.

Step 7: Repeat until the five-digit password is shown on the gauge display.

Step 8: Press ENTER.

Note: to erase password at any time while in the SETPW (set password) mode, press the ZERO/CLEAR key. The user will be prompted to reprogram the password once the five-digit password is entered. The gauge will display SAVE.

Step 9: Press Enter to save the password setting.

ENTPW: Once a user password has been established and entry into the CONFIG mode is required, the user will be prompted to ENTPW or enter password.

Follow setup steps 4-8 above.

RECAL: or recalibrate allows for zero, mid-scale, full-scale and factory default calibration of the gauge. The RECAL feature also allows for recalibration of gauges with 4-20mA output.

* Indicates default.

MENU FUNCTIONS

To use RECAL option:

Step 1: Press the Menu key on the keypad

Step 2: Press the ▲ (up arrow key) or ▼ (down arrow key) on the keypad until the word CONFIG appears.

Step 3: Press Enter.

Step 4: Enter user password if it has been programmed.

Step 5: Press ▲ (up arrow key) or ▼ (down arrow key) until the word RECAL appears.

Step 6: Press Enter.

Step 7: The gauge will now flash between INPUT and unit of measure on the lower line and .00 on the top line. Apply zero pressure to the gauge.

Step 8: Press Enter. Zero pressure is now set.

Step 9: The gauge will display full-scale pressure. Apply full-scale pressure to the gauge.

Step 10: Press Enter. Full-scale pressure is now set.

Step 11: The gauge will now display mid-scale pressure. Apply mid-scale pressure to the gauge.

Step 12: Press Enter. Mid-scale pressure is now set.

(Note: For compound ranges this recalibration is zero, full-scale, mid-scale and full-vac.)

FOR FACTORY CALIBRATED SETTINGS:

Step 13: To reinstate factory calibrated settings for zero, full-scale and mid-scale press the ▼ (down arrow key) Menu key until the word FACT appears.

Step 14: Press Enter. Factory calibration settings are now reinstated.

Step 15: After zero, full-scale and/or mid-scale or factory default calibration have been set, the word SAVE appears on the gauge display.

Step 16: Press Enter to finalize calibration.

*Indicates default.

MENU FUNCTIONS

Note: Calibration of Zero, mid-scale or span can be set independently of each other. For instance, if only full-scale calibration is required, press the ▼ (down arrow key) until the gauge display indicates full-scale pressure. Press Enter and proceed as indicated above. Calibration of zero, midscale and full-scale is recommended when recalibrating the gauge.

ZERO KEY (0bUTN): This feature allows the user to select percent of full-scale at which the gauge can be rezeroed using the Zero/Clear key on the keypad. Options include 5% full-scale*, 10% full-scale or DISAB (disable of the zero key).

To use ZERO option:

Step 1: Press the Menu key on the keypad.

Step 2: Press the ▲ (up arrow key) or ▼ (down arrow key) until the word CONFIG appears.

Step 3: Press Enter.

Step 4: Enter user password, if it has been programmed.

Step 5: Press the ▲ (up arrow key) or ▼ (down arrow key) until the word 0bUTN (zero key) appears.

Step 6: Press Enter.

Step 7: Press the ▲ (up arrow key) or ▼ (down arrow key) to select 5PCT (5% full-scale), dISAb (disable zero key) or 10PCT (10% full-scale).

Step 8: Press Enter to finalize the selection.

DISAB: or disable: This feature allows the user to dISAb (or disable) or ENAb (enable) items in the MENU. Some keypad keys can also be enabled or disabled. Any or all MENU items can be enabled or disabled.

To use DISAB option:

Step 1: Press the Menu key on the keypad.

Step 2: Press the ▲ (up arrow key) or ▼ (down arrow key) until the word dISAb appears.

*Indicates default.

MENU FUNCTIONS

Step 3: press ENTER. The current setting (ENAB or dISAB) will be displayed.

Step 4: Press the ▲ (up arrow key) or ▼ (down arrow key) on the keypad to select a setting.

Step 5: Press ENTER To finalize the setting.

GRAPH: This option allows the user to change the BAR graph on the gauge display to correspond to any desired pressure within the pressure limits of the gauge. This option is useful when identifying a select portion of the full-scale range of the gauge. The default setting for the GRAPH is zero and full-scale pressure. For compound gauges, the default setting for zero is set at full-scale vacuum. Full-scale pressure is set at the positive pressure as displayed on the gauge keypad.

For gauges supplied with the 4-20mA output option, the default is 4mA equals 0% of the bar graph and 20 mA equals 100% of the bar graph.

Changing the bar graph to a pressure other than 0 and 100% of range will also change the 4-20mA output to correspond with the new bar graph pressures for 0 and 100%.

To use GRAPH option:

Step 1: Press the MENU key.

Step 2: Press the ▲ (up arrow key) or ▼ (down arrow key) on the keypad until the word GRAPH appears.

Step 3: Press ENTER . The gauge display will indicate the set full scale pressure range setting on the top line. The middle line indicates the bar graph at 100% of full-scale. The bottom line of the display will indicate SETFS to set the full-scale range as displayed by the bar graph and 4-20mA.

Step 4: Press the ▲ (up arrow key) or ▼ (down arrow key) on the keypad to increase or decrease gauge value at 100% of range.

*Indicates default.

MENU FUNCTIONS

Step 5: Press the ENTER key to finalize your choice. The gauge display will now display SET. After two seconds the screen will display the pressure value for 0% on the top line. The middle line indicates the bar graph at 100% of fullscale. The bottom line will display SET 0.

Step 6: Press the ▲ (up arrow key) or ▼ (down arrow key) on the keypad to increase or decrease gauge value at 0% of range.

Step 7: Press the ENTER key to finalize your choice. The new values for the bar graph and 4/20mA settings have now been saved.

OFF: This option sets the amount of time before the gauge will turn itself off. Offerings are Never*, 30MIN, 10MIN, 5MIN, 2 MIN.

To use the OFF option:

Step 1: Press the MENU key.

Step 2: Press the ▲ (up arrow key) or ▼ (down arrow key) until the word OFF appears.

Step 3: Press ENTER.

Step 4: Press the ▲ (up arrow key) or ▼ (down arrow key) to select the desired OFF time.

Step 5: Press the Enter key to finalize the OFF setting.

UPDATE: This option allows for changing the rate at which pressure is updated on the display screen. This feature is useful with rapid changes in process pressure that may cause flutter of the display. Options are 100ms*, 1 sec, 500ms and 200ms, updates per second or 100ms*.

Since customer processes vary, update rates should be selected based on the application.

To use the UPDATE option:

Step 1: Press the MENU key.

*Indicates default.

MENU FUNCTIONS

Step 2: Press the ▲ (up arrow key) or ▼ (down arrow key) until the word UPDATE appears.

Step 3: Press Enter.

Step 4: Press the ▲ (up arrow key) or ▼ (down arrow key) to select an update rate.

Step 5: Press ENTER to finalize the selection.

DAMP or dampening: with five different options, this mode allows for taking process pressure readings and averaging them. This option is particularly useful to stabilize minor process fluctuations. The options are NONE*, AVG 8, AVG 6, AVG 4, AVG 2.

Step 1: Press the MENU key until the word dAMP appears.

Step 2: Press Enter

Step 3: Press the ▲ (up arrow key) or ▼ (down arrow key) to select a dampening option.

Step 4: Press the ENTER key to finalize your Damp option.

(This Menu item is only seen on units with the switch option)

SWSET: Allows for setting switch setpoints. The gauge is offered with one or two SPDT switches. If (one) SPDT switch is ordered the menu option is SW1. If (two) SPDT switches are ordered, the MENU options are SW1 and SW2.

Step 1: Press the MENU key.

Step 2: Press the ▲ (up arrow key) or ▼ (down arrow key) on the keypad to select the switch to be set. (If two switches are present.)

Step 3: Press ENTER. The top line of the gauge display will indicate pressure at 60% of the full-scale gauge range* or the most recent switch setpoint. The middle line of the display will indicate a bar graph that displays the pressure position within the pressure range. The bottom line will display SETPT (blinking).

*Indicates default.

MENU FUNCTIONS

Note: Setpoints are limited to the full-scale pressure range of the gauge.

Step 4: Press the ▲ (up arrow key) or ▼ (down arrow key) on the keypad to increase or decrease switch set-point

Step 5: Press the ENTER key to finalize switch setpoint. The gauge will display SET. After two seconds, the top line will indicate RETRP pressure. The bottom line will read SET.

Step 6: Repeat above to set RETRP (retrip value) If the gauge is supplied with (one) setpoint, the screen will advance to the measurement mode. If (two) switches are supplied the display will advance to SW2.

Repeat the aforementioned if the gauge is supplied with two switches.

Notes: The bar graph will increase or decrease as any setpoint pressure is adjusted. The bar graph indicates switch setpoint position within the full-scale pressure range of the gauge.

The switch setpoint unit of pressure measurement corresponds with the current set unit of measure of the gauge. If gauge unit of measurement is changed after switch(es) is set, switch setpoint(s) will automatically be updated to correspond with revised unit of measurement. Switch deadband is the difference between the SETPT (setpoint) and the RETRP (retrip) pressure.

DIGITAL INDUSTRIAL GAUGE SPECIFICATIONS:

Type:	Battery: DPG9030, DPG9032 (3") DPG9045, DPG9046 (4.5") Loop: DPG9130, DPG9031 (3") DPG9145, DPG9146 (4.5") Line: DPG9230, DPG9231 (3") DPG9245, DPG9246
Accuracy:	.25% Full Scale, terminal point
Case Size:	3", 4½"
Case Material:	3" SS, 4½" fiberglass reinforced thermoplastic or black epoxy coated aluminum
Case Encl. Rating:	Weatherproof, IP65
Wetted Materials:	17-4 SS (sensor), 316SS (socket)
Socket Size:	¼ or ½ NPT, JIS, DIN, SAE, (½ NPT only with 4½" case, others on application)
Socket Location:	Lower, 3, 9 and 12 o'clock
Ranges:	Vac. thru 20,000 psi (see eng. units below for other units)
Operating Temp.:	14/140°F (10/60°C)
Storage Temp.:	-4/158°F (-20/70°C)
DISPLAY	
Type:	LCD
Display Digits:	Five (5)
Character Height:	3" .60", 4½" .88"
Backlite:	Optional
Bar Graph:	Yes
Battery Life:	3" >1000 hrs., 4½" >3600 hrs.
Agency Approvals:	CE, FM* (Intrinsically Safe Class1, Div 1), CSA and CENELEC *FM is not available with the following: 4½" polypropylene case, SPDT switch option(s) (XU1, U2) or Backlite (XBL) option)
KEYPAD FUNCTIONS	
On/Off:	Manually turns unit on and off (auto off options in menu)
Zero/Clear:	Zeros display or clears min. and max. values when displayed
Min/Max ▼ (down) Arrow Key:	Stores min and max values, arrow key allows for scrolling thru menu items
Menu Key:	Provides access to menu options
Backlite ▲ (up) Arrow Key: (Backlite optional)	Manually turns backlite on and off (auto off options in menu), arrow key allows for five menu options. ▲ (up) arrow key allows for scrolling thru menu options
Enter:	Selects items in the menu
MENU MODE	
Engineering Units:	10 units of measurement are available; psi, In. H ₂ O (with three temp. options: 20°C, 60°F, 4°C*), Ft. H ₂ O, mPa, mBar, kPa, kg/cm ² , Bar, inHg and mmHg
Configuration Mode (Config):	Allows for changes to default settings of gauge including zero disable feature
Bar Graph (Graph):	Allows for adjustment of bargraph and 4-20 (optional feature)
Auto Off (Off):	Allows for changes to auto off of gauge, five options: Never, 2 min., 5 min., 15 min., 30 min.
Update Rate (Update):	Four options: 100 ms, 200 ms, 500 ms, 1 sec
Dampening (Damp):	Six options: None, average, 2, 4, 6, 8 times per 100ms
Backlite:	Five options: Never, 10 sec., 30 sec., 1 min., 5 min.
Field Recalibration:	Allows for recalibration of zero, midscale and span (password protected)
OPTIONS	
4-20mA Display:	12-36 Vdc, mA with unlimited turndown (within gauge range)
Line Powered:	12-36 Vdc, 2VA max.
Switching*:	(1) or (2) SPDT switches, (max. contact 30Vdc, 1 amp, 125Vac .5 Amp, Switches adjustable to 100% of range

DIGITAL INDUSTRIAL GAUGE RANGES:

psi	Comp. (psi)	mmHg (press.)	in. Hg (press.)	In. H ₂ O	mm H ₂ O	mBar	ft. H ₂ O	mPa	kPa	Bar/ ksc
	-15/0/15	1500	60	800	60	250	30	6	200	2
	-15/0/30	2000	100	1000	100	300	60	10	300	4
	-15/0/60	3000	160		160	400	160	50	400	6
30	-15/0/100		200		200	500	200		600	10
60			300		300	600	300		800	16
100			400		400	1000	400		1000	25
160			600		600	1500	600		1600	40
200			800		800	2000	1000		2500	60
300			1000		1000	2500			4000	100
600			1600			4000			6000	160
800			2000			5000			8000	250
1000			3000							400
1500			6000							500
2000										800
3000										1000
5000										
8000										
10,000										
15,000										
20,000										



DISPLAY MESSAGES:

Display/Problem	Description	Action
No Battery Icon Display (applicable to gauges with batteries)	Gauge has <10% battery life left	Replace batteries
OFFSET (blinking)	Zero/Clear button pushed when pressure displayed is beyond set rezero pressure limit	Only rezero the gauge within limits of setting in Menu
Menu button disabled	Gauge is in Max/Min mode	Push Max/Min button until unit of measure is displayed on keypad
Unit of measure selected in Menu displays N/A	Resolution at full scale pressure range exceeds 50,000 counts	Choose another unit of measure
I can't set the password I want	00000 is not a valid password	Select a different password
I can't access items in the main Menu	Items that cannot be accessed have been disabled	Enable item(s) in the Menu. See Menu/CONFIG and diSAb or DISABLE

WIRING DIAGRAM

Loop Powered 4-20mA (Type DPG 9130, DPG 9131, DPG 9145, DPG 9146)

2 conductor, 20 AWG shielded

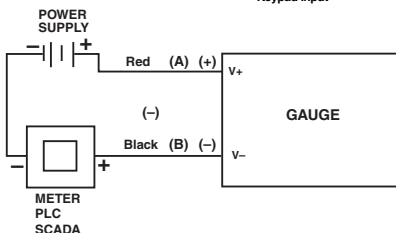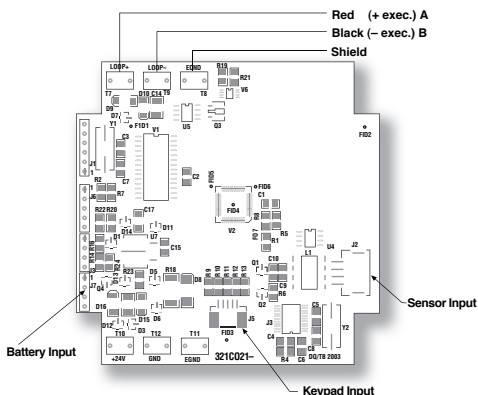


Installation Procedure

- ⚠ ESD precautions should be taken. See page 33 for details.
1. Ensure all power is off/disconnected from the circuit.
2. Connect the red wire (A) to the positive power terminal.
3. Connect the black wire (B) to the positive terminal on the meter.
4. Connect the negative side of the meter to the negative power terminal.

Note: Meter should be installed on the black wire only.

Load Limitations 4-20mA Output Only

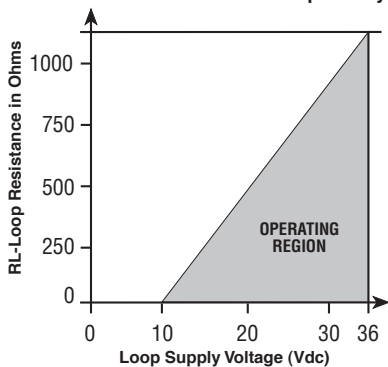

$$\mathbf{Vdc\ MIN = 12V + [0.022A \times (RL)]}$$

$$R_L = R_S + R_W$$

R_L = Loop Resistance (ohms)


R_S = Sense Resistance (ohms)

R_W = Wiring Resistance (ohms)

WIRING DIAGRAM

Line Powered (Type DPG 9230, DPG 9231, DPG 9245, DPG 9246)

2 conductor, 20 AWG shielded

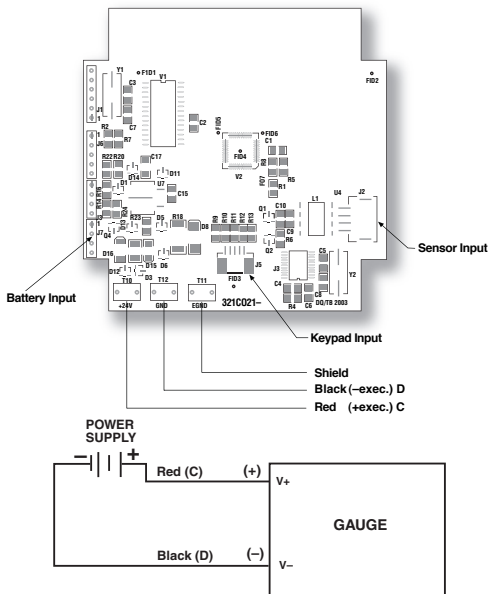



Installation Procedure

- ⚠** ESD precautions should be taken. See page 33 for details.
1. Ensure all power is off/disconnected from the circuit.
 2. Connect the red wire (C) to the positive power terminal.
 3. Connect the black wire (D) to the negative power terminal.

WIRING DIAGRAM

Line Powered with (1) SPDT switch (Type DPG 9230_-S1, DPG 9231_-S1, DPG 9245_-S1, DPG 9246_-S1)

5 conductor, 22 AWG shielded

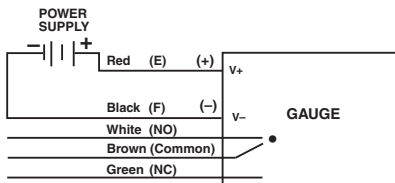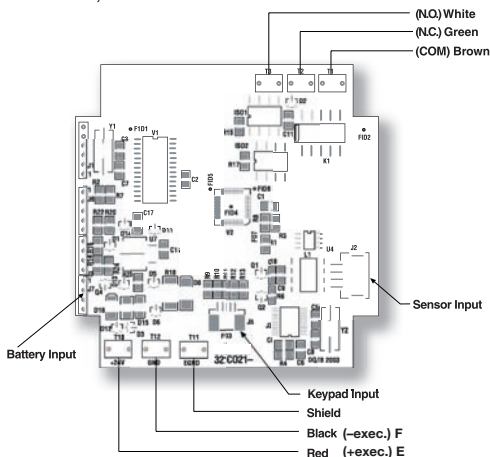

Installation Procedure

- ⚠ ESD precautions should be taken. See page 33 for details.
1. Ensure all power is off/disconnected from the circuit.
 2. Connect the red wire (E) to the positive power terminal.
 3. Connect the black wire (F) to the negative power terminal.

Wiring the Switch:



Normally Open: Use the white and brown wires.

Normally Closed: Use the green and brown wires.

WIRING DIAGRAM

Line Powered with (2) SPDT switches (Type DPG 9230_-S2, DPG 9231_-S2, DPG 9245_-S2, DPG 9246_-S2)

8 conductor, 22 AWG shielded

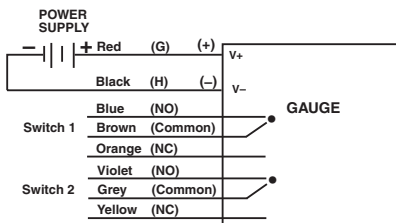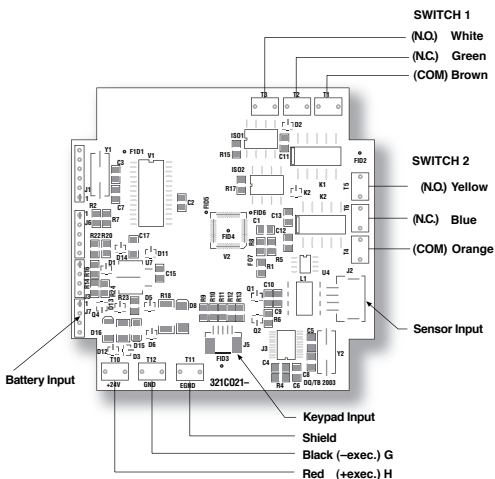

Installation Procedure



ESD precautions should be taken. See page 33 for details.

1. Ensure all power is off/disconnected from the circuit.
2. Connect the red wire (G) to the positive power terminal.
3. Connect the black wire (H) to the positive meter terminal.

Wiring Switch 1:

Normally Open: Use the white and brown wires.

Normally Closed: Use the green and brown wires.

Wiring Switch 2:



Normally Open: Use the yellow and orange wires.

Normally Closed: Use the blue and orange wires.

WIRING DIAGRAM

Line Powered/Loop Powered 4-20mA (Type DPG 9230_-A, DPG 9131_-A, DPG 9245_-A, DPG 9246_-A)

4 conductor, 20 AWG shielded

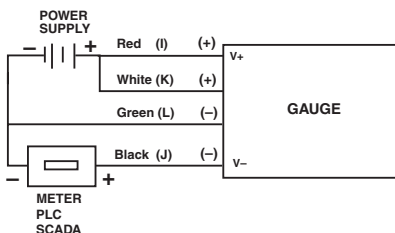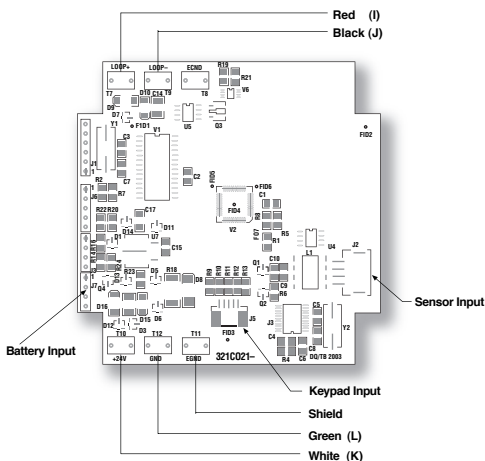

Installation Procedure

 ESD precautions should be taken. See page 33 for details.

1. Ensure all power is off/disconnected from the circuit.
2. Connect the white wire (K) to the positive power terminal.
3. Connect the green wire (L) to the negative power terminal.
4. Connect the red wire (I) to the positive power terminal.
5. Connect the black wire (J) to the positive meter terminal.
6. Connect the negative power terminal with the negative meter terminal.

Note: Meter should be installed on the black wire only.



If red/black wires are connected prior to the green/white and power is connected, output may be damaged due to overloading.

Warning: Using multiple power sources for line and loop power is not recommended as it may cause damage to the unit.

WIRING DIAGRAM

Line Powered/Loop Powered 4-20mA with (1) SPDT switch
(Type DPG 9230_-AS1, DPG 9231_-AS1, DPG 9245_-AS1,
DPG 9346_-AS1)

7 conductor, 22 AWG shielded

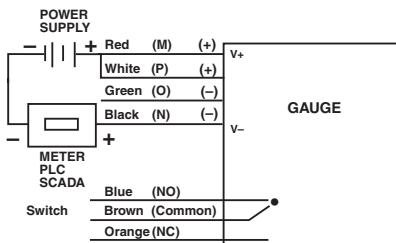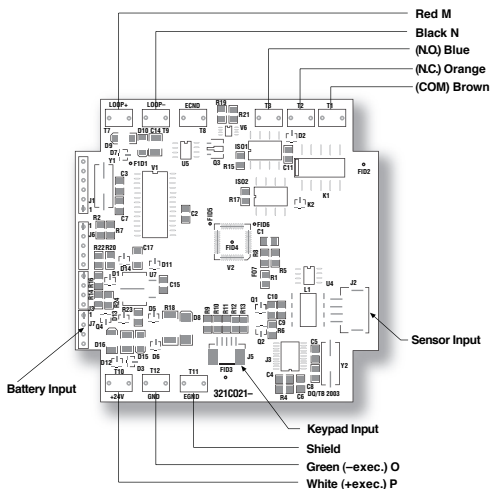

Installation Procedure

 ESD precautions should be taken. See page 33 for details.

1. Ensure all power is off/disconnected from the circuit.
2. Connect the white wire (P) to the positive power terminal.
3. Connect the green wire (O) to the negative power terminal.
4. Connect the red wire (M) to the positive power terminal.
5. Connect the black wire (N) to the positive meter terminal.
6. Connect the negative power terminal with the negative meter terminal.

Note: Meter should be installed on the black wire only.

If red/black wires are connected prior to the green/white and power is connected, output may be damaged due to overloading.


Wiring the Switch:

Normally Open: Use the blue and brown wires.

Normally Closed: Use the orange and brown wires.

WIRING DIAGRAM

Line Powered/Loop Powered 4-20mA with (2) SPDT switches
(Type DPG 9230_-AS2, DPG 9231_-AS2, DPG 9245_-AS2,
DPG 9246_-AS2) 10 conductor, 22 AWG shielded

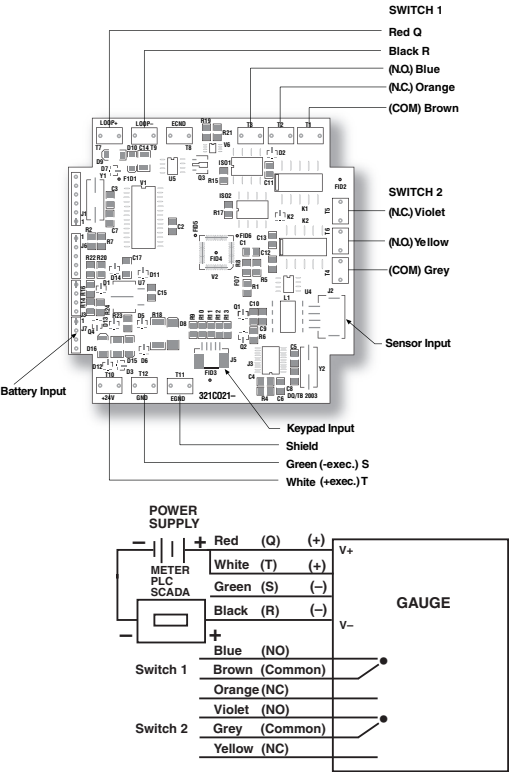

Installation Procedure

 ESD precautions should be taken. See page 33 for details.

1. Ensure all power is off/disconnected from the circuit.
2. Connect the white wire (T) to the positive power terminal.
3. Connect the green wire (S) to the negative power terminal.
4. Connect the red wire (Q) to the positive power terminal.
5. Connect the black wire (R) to the positive meter terminal.
6. Connect the negative power terminal with the negative meter terminal.

Note: Meter should be installed on the black wire only.

Wiring Switch 1:

Normally Open: Use the blue and brown wires.

Normally Closed: Use the orange and brown wires.

Wiring Switch 2:

Normally Open: Use the violet and grey wires.

Normally Closed: Use the yellow and grey wires.

GAUGE INSTALLATION:

The Ashcroft digital industrial gauge comes standard with either $\frac{1}{4}$ or $\frac{1}{2}$ NPT connection. Good piping practices recommend using teflon tape or a pipe sealant on the gauge threads. Utilize a $\frac{5}{16}$ " (3" case), $\frac{5}{8}$ " (4½" case) wrench on the wrench flat of the gauge to tighten the gauge to the process.

NEVER TIGHTEN GAUGE THREADS BY HOLDING THE BODY OF THE GAUGE. DOING SO MAY DAMAGE THE GAUGE AND MAKE THE GAUGE INOPERABLE.

Battery Installation and Replacement:

The Type 2074 comes standard with batteries installed. The 3" case uses qty (2) AA alkaline batteries, the 4½" case uses qty (2) C alkaline batteries. Use either Duracell MN2400, MX2400 or Energizer E92BP, X92RP AAA alkaline, non-rechargeable batteries.

Batteries have a life of approximately 1500 hours (3" case). 3600 hours (4½" case). Battery life is dependent on gauge usage, backlite settings and power off settings. When the lower bar of the battery icon of the gauge display flashes, the gauge has approximately 7 hours of life remaining.

To replace the batteries (3" case):

- 1) Remove the single screw on the back of the gauge case.
- 2) Hold the keypad in the palm of hand.
- 3) Carefully remove the two batteries from the holder and replace batteries. Use only AA alkaline non-rechargeable batteries

To replace the batteries (4½" case):

- 1) Remove the ring on the front of the gauge case.
- 2) Looking at the gauge case, carefully pull the front face out of the case.
- 3) Lay the gauge, face down on a flat surface.
- 4) Carefully remove the two batteries from the holder and replace the batteries. Use only C alkaline non-rechargeable batteries.

ESD PRECAUTIONS

Care should be taken to minimize exposure to ESD. Proper proto-call should be followed as outlined in:

ANSI/ESD S20.20-2007

ESD ADV1.0-2009

ANSI/ESD S541-2008

Additional ESD Precautions on Proper Handling:

Avoid carpets in cool, dry areas as well as other static generating materials such as plastic, cellophane, paper, or cardboard.

Leave digital gauges in their anti-static packaging until ready to be installed.

Dissipate static electricity before handling the digital gauge or using keypad by touching a well-grounded metal object, such as the system unit unpainted metal chassis.

If possible, use antistatic devices, such as wrist straps and floor mats.

When installing batteries, avoid touching (including clothing) the contacts and components.

When making wiring connection to digital gauge terminals, place digital gauge on grounded mat prior to making connection, and take care to avoid touching (including clothing) any components.

Take care when connecting or disconnecting cables. A damaged cable can cause a short in the electrical circuit.

When disconnecting a cable, always pull on the cable connector, case, or strain-relief loop, not on the cable itself.

Notes:

- 1) Do not mix ages or brands of batteries.
- 2) Do not replace batteries in hazardous areas.
- 3) To provide maximum battery life, replace both batteries
- 4) To provide maximum battery life, replace both batteries.

⚠ Pipe to which gauge is attached must be properly grounded.

PANEL MOUNTING DIMENSIONS:

