

# Technical Information

## Cerabar S

### PMC71, PMP71, PMP75

Process pressure measurement  
1-5 V DC, HART, PA, FF

Pressure transmitter with ceramic and metallic measuring cells



#### Applications

The device is used for the following measuring tasks:

- Absolute pressure and gauge pressure measurement in gases, steams or liquids in all areas of process engineering and process measurement technology
- Level, volume or mass measurements in liquids
- High process temperatures
  - up to 150 °C (302 °F) without diaphragm seal
  - up to 400 °C (752 °F) with typical diaphragm seals
- High pressures up to 700 bar (10 500 psi)
- Low-energy version with voltage output (1-5V DC), e.g. for operation on solar-operated control units (Remote Terminal Unit (RTU))

#### Your benefits

- Very good reproducibility and long-term stability
- High reference accuracy up to  $\pm 0.025$  %
- Turn down up to 100:1, higher on request
- Used for process pressure monitoring up to SIL 3, certified to IEC 61508 by TÜV SÜD
- High level of safety during operation thanks to function monitoring from the measuring cell to the electronics
- Easy electronics replacement guaranteed with HistoROM®/M-DAT

## Table of contents

|                                                                                                  |           |                                                                                                   |           |
|--------------------------------------------------------------------------------------------------|-----------|---------------------------------------------------------------------------------------------------|-----------|
| <b>About this document</b> .....                                                                 | <b>4</b>  | <b>Performance characteristics for measuring instruments with metallic process membrane</b> ..... | <b>32</b> |
| Document function .....                                                                          | 4         | Response time .....                                                                               | 32        |
| Symbols used .....                                                                               | 4         | Reference operating conditions .....                                                              | 32        |
| Documentation .....                                                                              | 5         | Total performance .....                                                                           | 32        |
| List of abbreviations .....                                                                      | 6         | Resolution .....                                                                                  | 35        |
| Turn down calculation .....                                                                      | 6         | Total error .....                                                                                 | 35        |
| Registered trademarks .....                                                                      | 6         | Long-term stability .....                                                                         | 36        |
| <b>Function and system design</b> .....                                                          | <b>8</b>  | Response time T63 and T90 .....                                                                   | 36        |
| Measuring principle .....                                                                        | 8         | Installation factors .....                                                                        | 38        |
| Product design .....                                                                             | 10        | <b>Mounting</b> .....                                                                             | <b>39</b> |
| Applications suitable for custody transfer measurement .....                                     | 10        | General installation instructions .....                                                           | 39        |
| Communication protocol .....                                                                     | 10        | Measuring arrangement for devices without diaphragm seals – PMC71, PMP71 .....                    | 39        |
| <b>Input</b> .....                                                                               | <b>11</b> | Measuring arrangement for devices with diaphragm seals – PMP75 .....                              | 39        |
| Measured variable .....                                                                          | 11        | Orientation .....                                                                                 | 39        |
| Measuring range .....                                                                            | 11        | Wall and pipe mounting, transmitter (optional) .....                                              | 40        |
| <b>Output</b> .....                                                                              | <b>14</b> | Wall and pipe mounting, valve manifold (optional) .....                                           | 40        |
| Output signal .....                                                                              | 14        | Heat insulation – PMC71 high-temperature version .....                                            | 40        |
| Signal range .....                                                                               | 14        | Mounting of PVDF screw-in fittings .....                                                          | 41        |
| Signal on alarm .....                                                                            | 14        | "Separate housing" version .....                                                                  | 42        |
| Load .....                                                                                       | 15        | Turning the housing .....                                                                         | 43        |
| Damping .....                                                                                    | 16        | <b>Environment</b> .....                                                                          | <b>44</b> |
| Alarm current .....                                                                              | 16        | Ambient temperature range .....                                                                   | 44        |
| Firmware version .....                                                                           | 16        | Storage temperature range .....                                                                   | 45        |
| Protocol-specific data HART .....                                                                | 16        | Degree of protection .....                                                                        | 45        |
| Wireless HART data .....                                                                         | 17        | Climate class .....                                                                               | 45        |
| Protocol-specific data PROFIBUS PA .....                                                         | 17        | Electromagnetic compatibility .....                                                               | 45        |
| Protocol-specific data FOUNDATION Fieldbus .....                                                 | 18        | Vibration resistance .....                                                                        | 45        |
| <b>Energy supply</b> .....                                                                       | <b>21</b> | Oxygen applications .....                                                                         | 46        |
| Terminal assignment .....                                                                        | 21        | PWIS-free applications .....                                                                      | 46        |
| Supply voltage .....                                                                             | 22        | Ultrapure gas applications .....                                                                  | 46        |
| Current consumption .....                                                                        | 23        | Hydrogen applications .....                                                                       | 46        |
| Electrical connection .....                                                                      | 23        | Operation in very corrosive environment .....                                                     | 46        |
| Terminals .....                                                                                  | 23        | <b>Process</b> .....                                                                              | <b>47</b> |
| Cable entries .....                                                                              | 23        | Process temperature limits .....                                                                  | 47        |
| Connectors .....                                                                                 | 24        | Process temperature limits of capillary armoring: PMP75 ..                                        | 48        |
| Cable specification .....                                                                        | 25        | Pressure specifications .....                                                                     | 49        |
| Start-up current .....                                                                           | 26        | <b>Mechanical construction</b> .....                                                              | <b>50</b> |
| Residual ripple .....                                                                            | 26        | Device height .....                                                                               | 50        |
| Overvoltage protection (optionally for HART, PROFIBUS PA and FOUNDATION Fieldbus) .....          | 26        | T14 housing, optional display on the side .....                                                   | 51        |
| Influence of power supply .....                                                                  | 26        | T17 housing (hygienic), optional display on the side .....                                        | 52        |
| <b>Performance characteristics for measuring instruments with ceramic process membrane</b> ..... | <b>27</b> | PMC71: height H .....                                                                             | 52        |
| Response time .....                                                                              | 27        | Explanation of terms .....                                                                        | 53        |
| Reference operating conditions .....                                                             | 27        | Process connections PMC71, internal process membrane ..                                           | 54        |
| Total performance .....                                                                          | 27        | Process connections PMC71, internal process membrane ..                                           | 56        |
| Resolution .....                                                                                 | 29        | Process connections PMC71, flush process membrane .....                                           | 57        |
| Total error .....                                                                                | 29        | Process connections PMC71, flush process membrane .....                                           | 58        |
| Long-term stability .....                                                                        | 29        | Process connections PMC71, flush process membrane .....                                           | 59        |
| Response time T63 and T90 .....                                                                  | 30        | Process connections PMC71, flush process membrane .....                                           | 62        |
| Installation factors .....                                                                       | 31        | PMC71 hygiene .....                                                                               | 63        |
|                                                                                                  |           | Process connections PMP71, internal process membrane ..                                           | 65        |
|                                                                                                  |           | Process connections PMP71, internal process membrane ..                                           | 66        |

|                                                            |            |                                                          |            |
|------------------------------------------------------------|------------|----------------------------------------------------------|------------|
| Process connections PMP71, internal process membrane . . . | 67         | Functional safety SIL/ IEC 61508 Declaration of          |            |
| Process connections PMP71, flush process membrane . . . .  | 68         | Conformity (optional) . . . . .                          | 121        |
| Process connections PMP71, flush process membrane . . . .  | 70         | CRN approval . . . . .                                   | 121        |
| Process connections PMP71, flush process membrane . . . .  | 71         | Pressure Equipment Directive 2014/68/EU (PED) . . . . .  | 121        |
| Process connections PMP71, flush process membrane . . . .  | 72         | MID Parts Certificate . . . . .                          | 122        |
| Process connections PMP71, flush process membrane . . . .  | 73         | Classification of process sealing between electrical     |            |
| Process connections PMP71, flush process membrane . . . .  | 74         | systems and (flammable or combustible) process fluids in |            |
| Process connections PMP71 . . . . .                        | 75         | accordance with ANSI/ISA 12.27.01 . . . . .              | 122        |
| Process connections PMP71 . . . . .                        | 75         | Inspection certificate . . . . .                         | 122        |
| Valve manifold DA63M- (optional) . . . . .                 | 76         |                                                          |            |
| PMP75 basic device . . . . .                               | 77         | <b>Ordering information . . . . .</b>                    | <b>124</b> |
| Process connections PMP75, flush process membrane . . . .  | 77         | Special device versions . . . . .                        | 124        |
| Process connections PMP75, flush process membrane . . . .  | 79         | Scope of delivery . . . . .                              | 124        |
| Process connections PMP75, flush TempC process             |            | Measuring point (TAG) . . . . .                          | 124        |
| membrane . . . . .                                         | 80         | Configuration data sheet . . . . .                       | 125        |
| Process connections PMP75, flush process membrane . . . .  | 81         |                                                          |            |
| Process connections PMP75, flush process membrane . . . .  | 82         | <b>Accessories . . . . .</b>                             | <b>127</b> |
| Hygienic process connections PMP75, flush process          |            | HistoROM®/M-DAT . . . . .                                | 127        |
| membrane . . . . .                                         | 83         | Welding flanges and weld-in adapters . . . . .           | 127        |
| Hygienic process connections PMP75, flush process          |            | Manifolds . . . . .                                      | 127        |
| membrane . . . . .                                         | 84         | Additional mechanical accessories . . . . .              | 127        |
| Hygienic process connections PMP75, flush process          |            | Service-specific accessories . . . . .                   | 127        |
| membrane . . . . .                                         | 85         |                                                          |            |
| Process connections PMP75, flush process membrane . . . .  | 88         | <b>Documentation . . . . .</b>                           | <b>128</b> |
| Process connections PMP75, flush process membrane . . . .  | 91         | Standard documentation . . . . .                         | 128        |
| Process connections PMP75 . . . . .                        | 95         | Supplementary device-dependent documentation . . . . .   | 128        |
| Separate housing: Wall and pipe mounting with mounting     |            |                                                          |            |
| bracket . . . . .                                          | 98         |                                                          |            |
| Flushing rings . . . . .                                   | 99         |                                                          |            |
| Weight . . . . .                                           | 99         |                                                          |            |
| Materials not in contact with process . . . . .            | 100        |                                                          |            |
| Materials in contact with process . . . . .                | 103        |                                                          |            |
| Fill fluid . . . . .                                       | 105        |                                                          |            |
|                                                            |            |                                                          |            |
| <b>Operability . . . . .</b>                               | <b>106</b> |                                                          |            |
| Operating concept . . . . .                                | 106        |                                                          |            |
| Local operation . . . . .                                  | 106        |                                                          |            |
| Remote operation . . . . .                                 | 109        |                                                          |            |
| HistoROM®/M-DAT (optional) . . . . .                       | 111        |                                                          |            |
| System integration . . . . .                               | 111        |                                                          |            |
|                                                            |            |                                                          |            |
| <b>Planning instructions for diaphragm seal</b>            |            |                                                          |            |
| <b>systems . . . . .</b>                                   | <b>112</b> |                                                          |            |
| Applications . . . . .                                     | 112        |                                                          |            |
| Design and operation mode . . . . .                        | 113        |                                                          |            |
| Diaphragm seal fill fluid . . . . .                        | 115        |                                                          |            |
| Information on cleaning . . . . .                          | 115        |                                                          |            |
| Installation instructions . . . . .                        | 115        |                                                          |            |
| Vacuum applications . . . . .                              | 119        |                                                          |            |
|                                                            |            |                                                          |            |
| <b>Certificates and approvals . . . . .</b>                | <b>120</b> |                                                          |            |
| CE mark . . . . .                                          | 120        |                                                          |            |
| RoHS . . . . .                                             | 120        |                                                          |            |
| RCM-Tick marking . . . . .                                 | 120        |                                                          |            |
| TSE (BSE) compliance (ADI free - Animal                    |            |                                                          |            |
| Derived Ingredients) . . . . .                             | 120        |                                                          |            |
| Ex approvals . . . . .                                     | 120        |                                                          |            |
| Corrosion test . . . . .                                   | 120        |                                                          |            |
| EAC conformity . . . . .                                   | 120        |                                                          |            |
| Suitable for hygiene applications . . . . .                | 120        |                                                          |            |
| Certificate of current Good Manufacturing Practices        |            |                                                          |            |
| (cGMP) . . . . .                                           | 120        |                                                          |            |

## About this document

### Document function

The document contains all the technical data on the device and provides an overview of the accessories and other products that can be ordered for the device.

### Symbols used

#### Safety symbols

| Symbol                                                                            | Meaning                                                                                                                                     |
|-----------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------|
|  | <b>DANGER!</b><br>This symbol alerts you to a dangerous situation. Failure to avoid this situation will result in serious or fatal injury.  |
|  | <b>WARNING!</b><br>This symbol alerts you to a dangerous situation. Failure to avoid this situation may result in serious or fatal injury.  |
|  | <b>CAUTION!</b><br>This symbol alerts you to a dangerous situation. Failure to avoid this situation may result in minor or moderate injury. |
|  | <b>NOTE!</b><br>This symbol contains information on procedures and other circumstances that do not result in personal injury.               |

#### Electrical symbols

| Symbol                                                                              | Meaning                                                                                                                         | Symbol                                                                               | Meaning                                                                                                                         |
|-------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------|
|  | <b>Protective ground connection</b><br>A terminal that must be connected to ground prior to establishing any other connections. |  | <b>Ground connection</b><br>A grounded terminal which, as far as the operator is concerned, is grounded via a grounding system. |

#### Symbols for certain types of Information

| Symbol                                                                              | Meaning                                                                  |
|-------------------------------------------------------------------------------------|--------------------------------------------------------------------------|
|  | <b>Permitted</b><br>Procedures, processes or actions that are permitted. |
|  | <b>Preferred</b><br>Procedures, processes or actions that are preferred. |
|  | <b>Forbidden</b><br>Procedures, processes or actions that are forbidden. |
|  | <b>Tip</b><br>Indicates additional information.                          |
|  | Reference to documentation                                               |
|  | Reference to page                                                        |
|  | Reference to graphic                                                     |
|  | Visual inspection                                                        |

### Symbols in graphics

| Symbol             | Meaning         |
|--------------------|-----------------|
| 1, 2, 3 ...        | Item numbers    |
| 1., 2., 3. ...     | Series of steps |
| A, B, C, ...       | Views           |
| A-A, B-B, C-C, ... | Sections        |

---

### Documentation

See the "Supplementary documentation" section →  128




The document types listed are available:

In the Download Area of the Endress+Hauser Internet site: [www.endress.com](http://www.endress.com) → Download

### Safety Instructions (XA)

See the "Safety instructions" section


## List of abbreviations

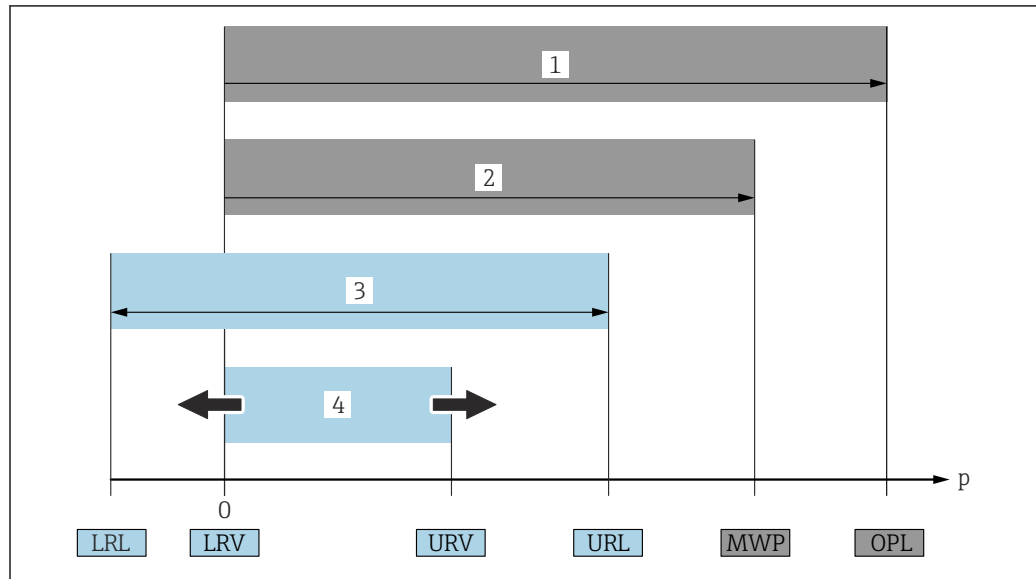

A0029505

- 1 OPL: The OPL (overpressure limit = measuring cell overload limit) for the device depends on the lowest-rated element, with regard to pressure, of the selected components, i.e. the process connection has to be taken into consideration in addition to the measuring cell. Pay attention to the pressure/temperature dependency.
  - 2 The MWP (maximum working pressure) for the measuring cells depends on the lowest-rated element, with regard to pressure, of the selected components, i.e. the process connection has to be taken into consideration in addition to the measuring cell. Pay attention to the pressure/temperature dependency. The MWP may be applied at the device for an unlimited period of time. The MWP can be found on the nameplate.
  - 3 The maximum measuring range corresponds to the span between the LRL and URL. This measuring range is equivalent to the maximum calibratable/adjustable span.
  - 4 The calibrated/adjusted span corresponds to the span between the LRV and URV. Factory setting: 0 to URL. Other calibrated spans can be ordered as customized spans.
- p Pressure  
 LRL Lower range limit  
 URL Upper range limit  
 LRV Lower range value  
 URV Upper range value  
 TD Turn down. Example - see the following section.

## Turn down calculation

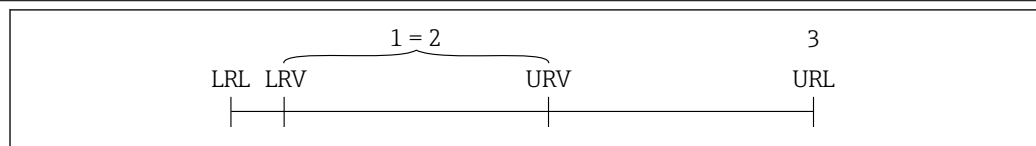

A0029545

- 1 Calibrated/adjusted span
- 2 Zero point-based span
- 3 Upper range limit

Example:

- Measuring cell: 10 bar (150 psi)
- Upper range limit (URL) = 10 bar (150 psi)
- Calibrated/adjusted span: 0 to 5 bar (0 to 75 psi)
- Lower range value (LRV) = 0 bar (0 psi)
- Upper range value (URV) = 5 bar (75 psi)

$$TD = \frac{URL}{|URV - LRV|}$$

In this example, the TD is therefore 2:1. This measuring span is based on the zero point.

## Registered trademarks

HART®

Registered trademark of the FieldComm Group, Austin, USA

**PROFIBUS®**

Registered trademark of the PROFIBUS User Organization, Karlsruhe, Germany


**FOUNDATION™Fieldbus**

Registered trademark of the FieldComm Group, Austin, Texas, USA

## Function and system design

### Measuring principle

#### Devices with ceramic process membrane (Ceraphire®)

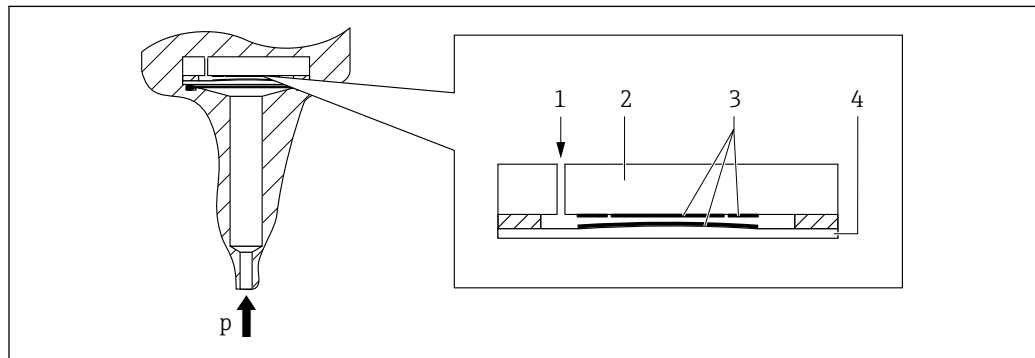

A0020465


- 1 Atmospheric pressure (gauge pressure measuring cells)
- 2 Ceramic substrate
- 3 Electrodes
- 4 Ceramic process membrane

The ceramic measuring cell is oil-free, i.e., the pressure acts directly on the robust ceramic process membrane and causes it to deflect. A pressure-dependent change in capacitance is measured at the electrodes of the ceramic substrate and the process membrane. The measuring range is determined by the thickness of the ceramic process membrane.

#### Advantages:

- Guaranteed overload resistance up to 40 times the nominal pressure (see "OPL" column in table) → 11)
- Thanks to ultrapure 99.9 % ceramic (Ceraphire®, see also "www.endress.com/ceraphire")
  - Extremely high chemical durability
  - High mechanical durability
- Suitable for vacuums
- Secondary containment for enhanced integrity
- Process temperatures up to 150 °C (302 °F)

#### Devices with metallic process membrane

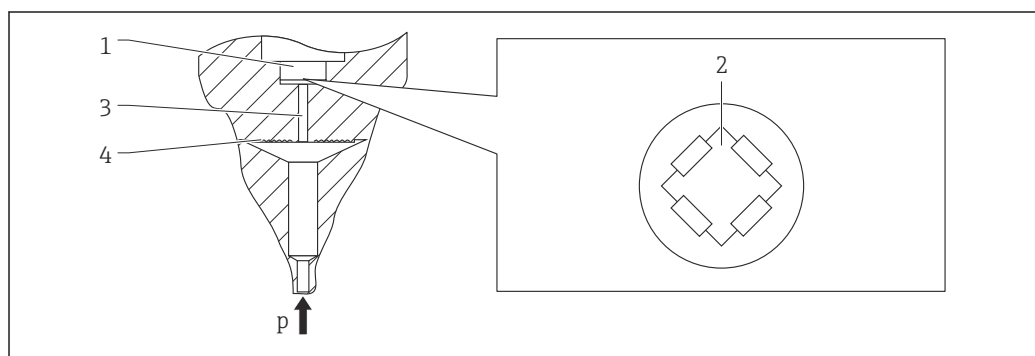

A0016448

- 1 Silicon measuring element, substrate
- 2 Wheatstone bridge
- 3 Channel with fill fluid
- 4 Metallic process membrane

#### PMP71

The process pressure deflects the metallic process membrane of the measuring cell and a fill fluid transfers the pressure to a Wheatstone bridge (semiconductor technology). The pressure-dependent change in the bridge output voltage is measured and evaluated.

**Advantages:**

- Can be used for process pressure up to 700 bar (10 500 psi)
- High long-term stability
- Guaranteed overload resistance up to 4 times the nominal pressure
- Secondary containment for enhanced integrity
- Significantly reduced thermal effect e.g. compared to diaphragm seal systems with capillaries

*PMP75*


The static pressure acts on the process membrane of the diaphragm seal and is transferred to the membrane of the measuring cell by a diaphragm seal fill fluid. The membrane is deflected and a fill fluid transfers the pressure to a resistance bridge. The pressure-dependent change in the bridge output voltage is measured and evaluated.

**Advantages:**

- Depending on the version, can be used for process pressures up to 400 bar (6 000 psi) and for extreme process temperatures
- High long-term stability
- Guaranteed overload resistance up to 4 times the nominal pressure
- Secondary containment for enhanced integrity

## Product design

## Level measurement (level, volume and mass):

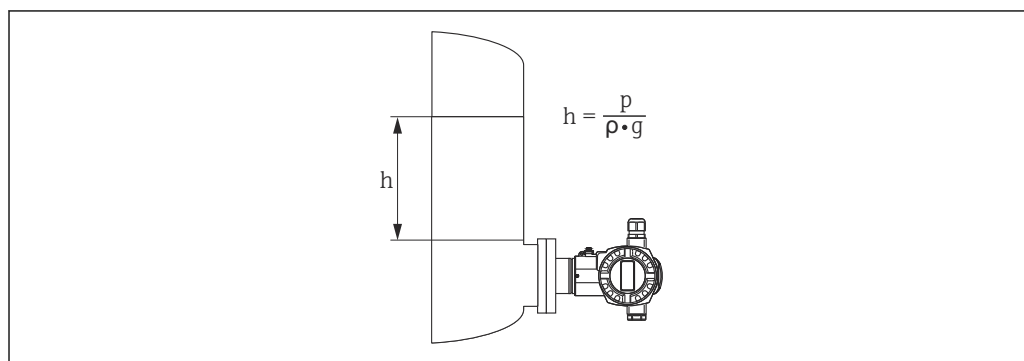

A0020466

*h* Height (level)  
*p* Pressure  
*ρ* Density of the medium  
*g* Gravitation constant

## Your benefits

- Selection of the level operating mode which is optimum for your application in the device software
- Volume and mass measurements in any vessel shape by means of a freely programmable characteristic curve
- Choice of diverse level units with automatic unit conversion
- A customized unit can be specified.
- Has a wide range of uses, e.g.
  - for foam formation
  - in vessels with agitators or screen fittings
  - for liquid gases

## Applications suitable for custody transfer measurement

The Parts Certificate is issued on the basis of the following standards:

- WELMEC guide 8.8 "General and Administrative Aspects of the Voluntary System of Modular Evaluation of Measuring instruments under the MID".
- OIML R117-1 Edition 2007 (E) "Dynamic measuring systems for liquids other than water".
- EN 12405-1/A1 Edition 2006 "Gas meters – Conversion devices – Part 1: Volume conversion".

## Communication protocol

- 4 to 20 mA with HART communication protocol
- PROFIBUS PA
  - Endress+Hauser devices meet the requirements specified by the FISCO model.
  - Due to a low current consumption of  $13 \text{ mA} \pm 1 \text{ mA}$ , the following number of devices can be operated on one bus segment if installing as per FISCO: up to 7 devices for Ex ia, CSA IS and FM IS applications or up to 27 devices for all other applications e.g. in non-hazardous areas, Ex nA etc. Further information on PROFIBUS PA can be found in Operating Instructions BA00034S "PROFIBUS DP/PA: Guidelines for planning and commissioning" and in the PNO Guideline.
- FOUNDATION Fieldbus
  - Endress+Hauser devices meet the requirements specified by the FISCO model.
  - Due to a low current consumption of  $15.5 \text{ mA} \pm 1 \text{ mA}$ , the following number of devices can be operated on one bus segment if installing as per FISCO: up to 6 devices for Ex ia, CSA IS and FM IS applications or up to 24 devices for all other applications e.g. in non-hazardous areas, Ex nA etc. Further information on FOUNDATION Fieldbus, such as requirements for bus system components, can be found in Operating Instructions BA00013S "FOUNDATION Fieldbus Overview".

## Input

### Measured variable

### Measured process variables

- Absolute pressure
- Gauge pressure

### Measuring range

### PMC71 - with ceramic process membrane (Ceraphire®) for gauge pressure

| Measuring cell      | Maximum measuring range |               | Smallest calibratable measuring span <sup>1)</sup> | MWP          | OPL      | Vacuum resistance                          | Option <sup>2)</sup> |
|---------------------|-------------------------|---------------|----------------------------------------------------|--------------|----------|--------------------------------------------|----------------------|
|                     | lower (LRL)             | upper (URL)   |                                                    |              |          |                                            |                      |
|                     | [bar (psi)]             | [bar (psi)]   |                                                    |              |          | [bar <sub>abs</sub> (psi <sub>abs</sub> )] |                      |
| 100 mbar (1.5 psi)  | -0.1 (-1.5)             | +0.1 (+1.5)   | 0.005 (0.075)                                      | 2.7 (40.5)   | 4 (60)   | 0.7 (10.5)                                 | 1C                   |
| 250 mbar (3.75 psi) | -0.25 (-3.75)           | +0.25 (+3.75) | 0.005 (0.075)                                      | 3.3 (49.5)   | 5 (75)   | 0.5 (7.5)                                  | 1E                   |
| 400 mbar (6 psi)    | -0.4 (-6)               | +0.4 (+6)     | 0.005 (0.075)                                      | 5.3 (79.5)   | 8 (120)  | 0                                          | 1F                   |
| 1 bar (15 psi)      | -1 (-15)                | +1 (+15)      | 0.01 (0.15)                                        | 6.7 (100.5)  | 10 (150) | 0                                          | 1H                   |
| 2 bar (30 psi)      | -1 (-15)                | +2 (+30)      | 0.02 (0.3)                                         | 12 (180)     | 18 (270) | 0                                          | 1K                   |
| 4 bar (60 psi)      | -1 (-15)                | +4 (+60)      | 0.04 (0.6)                                         | 16.7 (250.5) | 25 (375) | 0                                          | 1M                   |
| 10 bar (150 psi)    | -1 (-15)                | +10 (+150)    | 0.1 (1.5)                                          | 26.7 (400.5) | 40 (600) | 0                                          | 1P                   |
| 40 bar (600 psi)    | -1 (-15)                | +40 (+600)    | 0.4 (6)                                            | 40 (600)     | 60 (900) | 0                                          | 1S                   |

1) Turn down > 100:1 on request or can be set on device

2) Product Configurator, order code for "Sensor range; sensor over pressure limit"

### PMC71 - with ceramic process membrane (Ceraphire®) for absolute pressure

| Measuring cell      | Maximum measuring range                    |                                            | Smallest calibratable measuring span <sup>1)</sup> | MWP          | OPL      | Vacuum resistance | Option <sup>2)</sup> |
|---------------------|--------------------------------------------|--------------------------------------------|----------------------------------------------------|--------------|----------|-------------------|----------------------|
|                     | lower (LRL)                                | upper (URL)                                |                                                    |              |          |                   |                      |
|                     | [bar <sub>abs</sub> (psi <sub>abs</sub> )] | [bar <sub>abs</sub> (psi <sub>abs</sub> )] |                                                    |              |          |                   |                      |
| 100 mbar (1.5 psi)  | 0                                          | +0.1 (+1.5)                                | 0.005 (0.075)                                      | 2.7 (40.5)   | 4 (60)   | 0                 | 2C                   |
| 250 mbar (3.75 psi) | 0                                          | +0.25 (+3.75)                              | 0.005 (0.075)                                      | 3.3 (49.5)   | 5 (75)   | 0                 | 2E                   |
| 400 mbar (6 psi)    | 0                                          | +0.4 (+6)                                  | 0.005 (0.075)                                      | 5.3 (79.5)   | 8 (120)  | 0                 | 2F                   |
| 1 bar (15 psi)      | 0                                          | +1 (+15)                                   | 0.01 (0.15)                                        | 6.7 (100.5)  | 10 (150) | 0                 | 2H                   |
| 2 bar (30 psi)      | 0                                          | +2 (+30)                                   | 0.02 (0.3)                                         | 12 (180)     | 18 (270) | 0                 | 2K                   |
| 4 bar (60 psi)      | 0                                          | +4 (+60)                                   | 0.04 (0.6)                                         | 16.7 (250.5) | 25 (375) | 0                 | 2M                   |
| 10 bar (150 psi)    | 0                                          | +10 (+150)                                 | 0.1 (1.5)                                          | 26.7 (400.5) | 40 (600) | 0                 | 2P                   |
| 40 bar (600 psi)    | 0                                          | +40 (+600)                                 | 0.4 (6)                                            | 40 (600)     | 60 (900) | 0                 | 2S                   |

1) Turn down > 100:1 on request or can be set on device

2) Product Configurator, order code for "Sensor range; sensor over pressure limit"

### PMP71 and PMP75 – metallic process membrane for gauge pressure

| Measuring cell                     | Maximum measuring range |               | Smallest calibratable measuring span <sup>1)</sup> | MWP          | OPL                      | Vacuum resistance <sup>2)</sup>            | Option <sup>3)</sup> |
|------------------------------------|-------------------------|---------------|----------------------------------------------------|--------------|--------------------------|--------------------------------------------|----------------------|
|                                    | lower (LRL)             | upper (URL)   |                                                    |              |                          | Silicone oil/<br>Inert oil                 |                      |
|                                    | [bar (psi)]             | [bar (psi)]   |                                                    |              |                          | [bar <sub>abs</sub> (psi <sub>abs</sub> )] |                      |
| 400 mbar (6 psi)                   | -0.4 (-6)               | +0.4 (+6)     | 0.005 (0.075)                                      | 4 (60)       | 6 (90)                   | 0.01/0.04 (0.15/0.6)                       | 1F                   |
| 1 bar (15 psi)                     | -1 (-15)                | +1 (+15)      | 0.01 (0.15)                                        | 6.7 (100)    | 10 (150)                 |                                            | 1H                   |
| 2 bar (30 psi)                     | -1 (-15)                | +2 (+30)      | 0.02 (0.3)                                         | 13.3 (200)   | 20 (300)                 |                                            | 1K                   |
| 4 bar (60 psi)                     | -1 (-15)                | +4 (+60)      | 0.04 (0.6)                                         | 18.7 (280.5) | 28 (420)                 |                                            | 1M                   |
| 10 bar (150 psi)                   | -1 (-15)                | +10 (+150)    | 0.1 (1.5)                                          | 26.7 (400.5) | 40 (600)                 |                                            | 1P                   |
| 40 bar (600 psi)                   | -1 (-15)                | +40 (+600)    | 0.4 (6)                                            | 100 (1500)   | 160 (2400)               |                                            | 1S                   |
| 100 bar (1 500 psi)                | -1 (-15)                | +100 (+1500)  | 1.0 (15)                                           | 100 (1500)   | 400 (6000) <sup>4)</sup> |                                            | 1U                   |
| 400 bar (6 000 psi)                | -1 (-15)                | +400 (+6000)  | 4.0 (60)                                           | 400 (6000)   | 600 (9000)               |                                            | 1W                   |
| 700 bar (10 500 psi) <sup>5)</sup> | -1 (-15)                | +700 (+10500) | 7.0 (105)                                          | 700 (10500)  | 1050 (15750)             |                                            | 1X                   |

- 1) Turn down > 100:1 on request or can be set on device
- 2) The vacuum resistance applies for the measuring cell under reference operating conditions. A ceramic process membrane is recommended for applications in the limit range. The pressure and temperature application limits of the selected fill fluid must also be observed for the PMP75 → 115.
- 3) Product Configurator, order code for "Sensor range; sensor over pressure limit"
- 4) If the option "JN" is ordered in the order code for "Test, Certificate", then the OPL is 160 bar (2 400 psi).
- 5) PMP71 only, PMP75 on request

### PMP71 and PMP75 – metallic process membrane for absolute pressure

| Measuring cell                     | Maximum measuring range <sup>1)</sup>      |                                            | Smallest calibratable measuring span <sup>2)</sup> | MWP          | OPL                      | Vacuum resistance <sup>3)</sup>            | Option <sup>4)</sup> |
|------------------------------------|--------------------------------------------|--------------------------------------------|----------------------------------------------------|--------------|--------------------------|--------------------------------------------|----------------------|
|                                    | lower (LRL)                                | upper (URL)                                |                                                    |              |                          | Silicone oil/<br>Inert oil                 |                      |
|                                    | [bar <sub>abs</sub> (psi <sub>abs</sub> )] | [bar <sub>abs</sub> (psi <sub>abs</sub> )] |                                                    |              |                          | [bar <sub>abs</sub> (psi <sub>abs</sub> )] |                      |
| 400 mbar (6 psi)                   | 0                                          | +0.4 (+6)                                  | 0.005 (0.075)                                      | 4 (60)       | 6 (90)                   | 0.01/0.04 (0.15/0.6)                       | 2F                   |
| 1 bar (15 psi)                     | 0                                          | +1 (+15)                                   | 0.01 (0.15)                                        | 6.7 (100)    | 10 (150)                 |                                            | 2H                   |
| 2 bar (30 psi)                     | 0                                          | +2 (+30)                                   | 0.02 (0.3)                                         | 13.3 (200)   | 20 (300)                 |                                            | 2K                   |
| 4 bar (60 psi)                     | 0                                          | +4 (+60)                                   | 0.04 (0.6)                                         | 18.7 (280.5) | 28 (420)                 |                                            | 2M                   |
| 10 bar (150 psi)                   | 0                                          | +10 (+150)                                 | 0.1 (1.5)                                          | 26.7 (400.5) | 40 (600)                 |                                            | 2P                   |
| 40 bar (600 psi)                   | 0                                          | +40 (+600)                                 | 0.4 (6)                                            | 100 (1500)   | 160 (2400)               |                                            | 2S                   |
| 100 bar (1 500 psi)                | 0                                          | +100 (+1500)                               | 1.0 (15)                                           | 100 (1500)   | 400 (6000) <sup>5)</sup> |                                            | 2U                   |
| 400 bar (6 000 psi)                | 0                                          | +400 (+6000)                               | 4.0 (60)                                           | 400 (6000)   | 600 (9000)               |                                            | 2W                   |
| 700 bar (10 500 psi) <sup>6)</sup> | 0                                          | +700 (+10500)                              | 7.0 (105)                                          | 700 (10500)  | 1050 (15750)             |                                            | 2X                   |

- 1) PMP75: Within the measuring range, the minimum upper range value of 80 mbar<sub>abs</sub> (1.16 psi<sub>abs</sub>) must be observed.
- 2) Turn down > 100:1 on request or can be set on device
- 3) The vacuum resistance applies for the measuring cell under reference operating conditions. A ceramic process membrane is recommended for applications in the limit range. The pressure and temperature application limits of the selected fill fluid must also be observed for the PMP75 → 115.
- 4) Product Configurator, order code for "Sensor range; sensor over pressure limit"
- 5) If the option "JN" is ordered in the order code for "Test, Certificate", then the OPL is 160 bar (2 400 psi).
- 6) PMP71 only, PMP75 on request

**PMP71 - metallic process membrane for absolute pressure with MID parts certificate**

| Measuring cell | Maximum measuring range                    |                                            | Min. WP for gas applications suitable for custody transfer measurement | Min. WP for liquid applications suitable for custody transfer measurement | MWP                                        | OPL                                        | Vacuum resistance <sup>1)</sup> | Option <sup>2)</sup> |
|----------------|--------------------------------------------|--------------------------------------------|------------------------------------------------------------------------|---------------------------------------------------------------------------|--------------------------------------------|--------------------------------------------|---------------------------------|----------------------|
|                | lower (LRL) <sup>3)</sup>                  | upper (URL) <sup>4)</sup>                  |                                                                        |                                                                           |                                            |                                            | Silicone oil/<br>Inert oil      |                      |
| [bar (psi)]    | [bar <sub>abs</sub> (psi <sub>abs</sub> )] | [bar <sub>abs</sub> (psi <sub>abs</sub> )] | [bar (psi)]                                                            | [bar (psi)]                                                               | [bar <sub>abs</sub> (psi <sub>abs</sub> )] | [bar <sub>abs</sub> (psi <sub>abs</sub> )] | [bar (psi)]                     |                      |
| 10 (150)       | 0                                          | +10 (150)                                  | 0.5 (7.5)                                                              | 0.5 (7.5)                                                                 | 26.7 (400.5)                               | 40 (600)                                   | 0.01/0.04 (0.15/1)              | MP                   |
| 50 (750)       | 0                                          | +50 (750)                                  | 10 (150)                                                               | 2.5 (37.5)                                                                | 100 (1500)                                 | 400 (6000)                                 | 0.01/0.04 (0.15/1)              | MT                   |
| 100 (1500)     | 0                                          | +100 (1500)                                | 5 (75)                                                                 | 5 (75)                                                                    | 100 (1500)                                 | 400 (6000)                                 | 0.01/0.04 (0.15/1)              | MU                   |

1) The vacuum resistance applies to the measuring cell under reference operating conditions

2) Product Configurator, order code for "Sensor range; sensor over pressure limit"


3) By default, the device is set to a lower measuring range of 0 bar. Please specify when ordering if the lower measuring range is to be set to a different default value.

4) Max. WP (working pressure) for gas and liquid applications suitable for custody transfer measurement

## Output

### Output signal

- 4 to 20 mA with superimposed digital communication protocol HART, 2-wire
- 1-5V DC, 3-wire
- Digital communication signal PROFIBUS PA (Profile 3.0), 2-wire
  - Signal coding: Manchester Bus Powered (MBP): Manchester II
  - Transmission rate: 31.25 KBit/s voltage mode
- Digital communication signal FOUNDATION Fieldbus, 2-wire
  - Signal coding: Manchester Bus Powered (MBP): Manchester II
  - Transmission rate: 31.25 KBit/s voltage mode
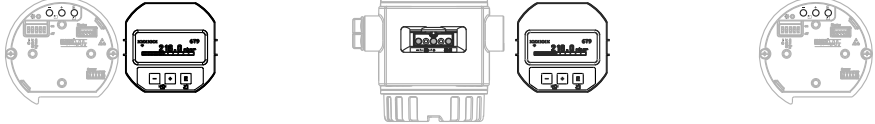
| Output               | Internal + LCD                                                                     | External + LCD | Internal |
|----------------------|------------------------------------------------------------------------------------|----------------|----------|
|                      |  |                |          |
|                      | Option <sup>1)</sup>                                                               |                |          |
| 4 to 20mA HART       | B                                                                                  | A              | C        |
| 4 to 20mA HART, Li=0 | E                                                                                  | D              | F        |
| 1-5V DC              | H                                                                                  | G              | -        |
| PROFIBUS PA          | N                                                                                  | M              | O        |
| FOUNDATION Fieldbus  | Q                                                                                  | P              | R        |

1) Product Configurator, order code for "Display, operation:"

### Signal range

#### 4 to 20 mA

3.8 mA to 20.5 mA

#### 1-5V DC

0.95 to 5.125 V

### Signal on alarm

#### 4 to 20 mA HART

As per NAMUR NE43.

- Max. alarm: can be set from 21 to 23 mA (factory setting: 22 mA)
- Hold measured value: last measured value is held
- Min. alarm: 3.6 mA

#### 1-5V DC

- Max. alarm: can be set from 5.25 to 5.75 V
- Min. Alarm: 0.9 V

#### PROFIBUS PA

As per NAMUR NE43.

Can be set in the Analog Input Block.

Options:

- Last Valid Out Value (factory setting)
- Fail Safe Value
- Status bad

#### FOUNDATION Fieldbus

As per NAMUR NE43.

Can be set in the Analog Input Block.


Options:

- Last Good Value
- Fail Safe Value (factory setting)
- Wrong Value

## Load

### 4 to 20 mA HART

In order to guarantee sufficient terminal voltage in two-wire devices, a maximum load resistance  $R$  (including line resistance) must not be exceeded depending on the supply voltage  $U_0$  of the supply unit. In the following load diagrams, observe the position of the jumper and the explosion protection:

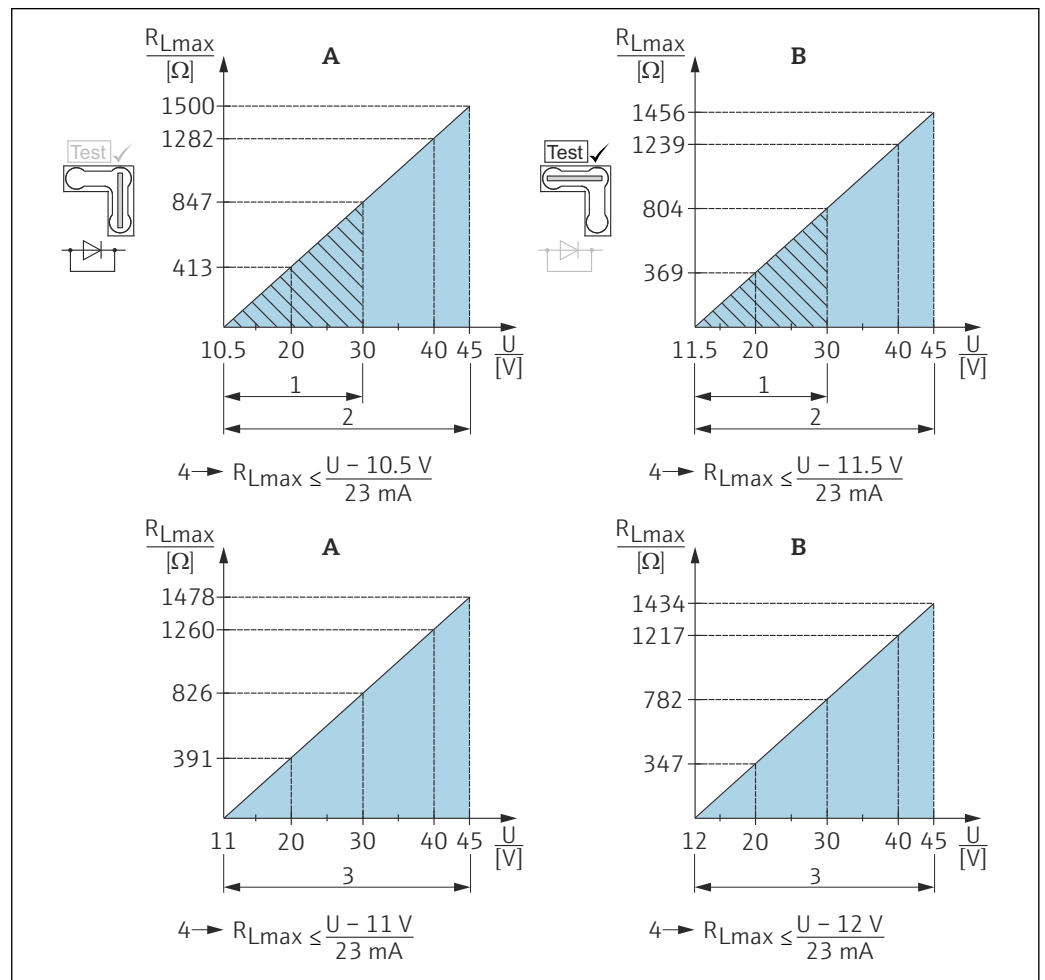

A Jumper for 4 to 20 mA test signal set to "Non-test" position

B Jumper for 4 to 20 mA test signal set to "Test" position

1 Power supply 10.5 (11.5) to 30 V DC for 1/2 G, 1 GD, 1/2 GD, FM IS, CSA IS, IECEx ia, NEPSI Ex ia

2 Power supply 10.5 (11.5) to 45 V DC for devices for non-hazardous areas, 1/2 D, 1/3 D, 2 G Ex d, 3 G Ex nA, FM XP, FM DIP, FM NI, CSA XP, CSA dust ignition-proof, NEPSI Ex d

3 Power supply 11 (12) to 45 V DC for PMC71, Ex d[ia], NEPSI Ex d[ia]

4  $R_{Lmax}$  maximum load resistance

U Supply voltage



When operating via a handheld terminal or via a PC with an operating program, a minimum communication resistance of 250 Ω must be taken into account.

### 1-5V DC

The load must be at least 100 kΩ.

**Damping**

A damping affects all outputs (output signal, display):

- via local display, handheld terminal or PC (handheld terminal or PC not for 1-5V DC) with operating program, continuous from 0 to 999 s
- Also for HART and PROFIBUS PA: Via DIP switch on the electronic insert, switch position "on" = set value and "off"
- 1-5V DC: via DIP switch on electronic insert switch position "on" = set value and "off"
- Factory setting: 2 s

**Alarm current**

| Designation                            | Option <sup>1)</sup> |
|----------------------------------------|----------------------|
| Min alarm current                      | J                    |
| HART burst mode PV                     | J                    |
| Min alarm current + HART burst mode PV | J                    |

1) Product Configurator, order code for "Additional options 1" and "Additional options 2"

**Firmware version**

| Designation                     | Option <sup>1)</sup> |
|---------------------------------|----------------------|
| 02.20.zz, HART 7, DevRev22      | 72                   |
| 02.11.zz, HART 5, DevRev21      | 73                   |
| 04.00.zz, FF, DevRev07          | 74                   |
| 04.01.zz, PROFIBUS PA, DevRev03 | 75                   |
| 02.10.zz, HART 5, DevRev21      | 76                   |
| 03.00.zz, FF, DevRev06          | 77                   |
| 04.00.zz, PROFIBUS PA           | 78                   |
| 02.30.zz, HART 7                | 71                   |

1) Product Configurator, order code for "Firmware version"

**Protocol-specific data HART**

|                                    |                                                                                                                                                                                                                     |
|------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Manufacturer ID                    | 17 (11 hex)                                                                                                                                                                                                         |
| Device type ID                     | 24 (18 hex)                                                                                                                                                                                                         |
| Device revision                    | <ul style="list-style-type: none"> <li>■ 21 (15 hex) - SW version 02.1y.zz - HART specification 5</li> <li>■ 22 (16 hex) - SW version 02.2y.zz - HART specification 7</li> </ul>                                    |
| HART specification                 | <ul style="list-style-type: none"> <li>■ 5</li> <li>■ 7</li> </ul>                                                                                                                                                  |
| DD revision                        | <ul style="list-style-type: none"> <li>■ 4 (Russian in language selection) for device revision 21</li> <li>■ 3 (Dutch in language selection) for device revision 21</li> <li>■ 1 for device revision 22</li> </ul>  |
| Device description files (DTM, DD) | Information and files under: <ul style="list-style-type: none"> <li>■ <a href="http://www.endress.com">www.endress.com</a></li> <li>■ <a href="http://www.fieldcommgroup.org">www.fieldcommgroup.org</a></li> </ul> |
| HART load                          | Min. 250 Ω                                                                                                                                                                                                          |

|                       |                                                                                                                                                                                                                                                                                                                                                                                                          |
|-----------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| HART device variables | <p>The measured values are assigned to the device variables as follows:</p> <p><b>Measured values for PV (primary variable)</b></p> <ul style="list-style-type: none"> <li>■ Pressure</li> <li>■ Level</li> <li>■ Tank content</li> </ul> <p><b>Measured values for SV, TV (second and third variable)</b></p> <p>Pressure</p> <p><b>Measured values for QV (fourth variable)</b></p> <p>Temperature</p> |
| Supported functions   | <ul style="list-style-type: none"> <li>■ Burst mode</li> <li>■ Additional transmitter status</li> <li>■ Device locking</li> <li>■ Alternative measuring modes</li> </ul>                                                                                                                                                                                                                                 |

**Wireless HART data**

|                           |                                                                               |
|---------------------------|-------------------------------------------------------------------------------|
| Minimum starting voltage  | 11.5 V (default) or 10.5 V if jumper not set to "Test" position <sup>1)</sup> |
| Start-up current          | 12 mA                                                                         |
| Starting time             | 10 s                                                                          |
| Minimum operating voltage | 11.5 V (default) or 10.5 V if jumper not set to "Test" position <sup>1)</sup> |
| Multidrop current         | 4 mA                                                                          |
| Time for connection setup | 1 s                                                                           |

1) Or higher if operating near the ambient temperature limits (−40 to +85 °C (−40 to +185))

**Protocol-specific data  
PROFIBUS PA**

|                       |                                                                                                                                                                                                                                                                                                       |
|-----------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Manufacturer ID       | 17 (11 hex)                                                                                                                                                                                                                                                                                           |
| Identification number | 1541 hex                                                                                                                                                                                                                                                                                              |
| Profile version       | <p>3.0</p> <ul style="list-style-type: none"> <li>■ SW version 03.00.zz</li> <li>■ SW version 04.00.zz</li> </ul> <p>3.02</p> <p>SW version 04.01.zz ( device revision 3)</p> <p>Compatibility with SW version 03.00.zz and higher.</p>                                                               |
| GSD revision          | <ul style="list-style-type: none"> <li>■ 4 (SW version 3.00.zz and 4.00.zz)</li> <li>■ 5 (device revision 3)</li> </ul>                                                                                                                                                                               |
| DD revision           | <ul style="list-style-type: none"> <li>■ 1 (SW version 3.00.zz and 4.00.zz)</li> <li>■ 1 (device revision 3)</li> </ul>                                                                                                                                                                               |
| GSD file              | Information and files under:                                                                                                                                                                                                                                                                          |
| DD files              | <ul style="list-style-type: none"> <li>■ <a href="http://www.endress.com">www.endress.com</a></li> <li>■ <a href="http://www.profibus.org">www.profibus.org</a></li> </ul>                                                                                                                            |
| Output values         | <p><b>Measured values for PV (via Analog Input Function Block)</b></p> <ul style="list-style-type: none"> <li>■ Pressure</li> <li>■ Level</li> <li>■ Tank content</li> </ul> <p><b>Measured values for SV</b></p> <ul style="list-style-type: none"> <li>■ Pressure</li> <li>■ Temperature</li> </ul> |

|                     |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
|---------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Input values        | Input value sent from PLC, can be shown on display                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   |
| Supported functions | <ul style="list-style-type: none"> <li>Identification &amp; maintenance, simplest device identifier on the control system and nameplate</li> <li>Condensed status (only with Profile Version 3.02)</li> <li>Automatic ID number adjustment and switchable to the following ID numbers (only with Profile Version 3.02): <ul style="list-style-type: none"> <li>9700: Profile-specific transmitter identification number with the "Classic" or "Condensed" status.</li> <li>1501: Compatibility mode for the old Cerabar S generation (PMC731, PMP731, PMC631, PMP635).</li> <li>1541: Identification number of the new Cerabar S generation (PMC71, PMP71, PMP75).</li> </ul> </li> <li>Device locking: The device can be locked by hardware or software.</li> </ul> |

#### Protocol-specific data FOUNDATION Fieldbus

|                                            |                                                                                                                                                                                                                                                                                   |
|--------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Manufacturer ID                            | 452B48 hex                                                                                                                                                                                                                                                                        |
| Device type                                | 1007 hex                                                                                                                                                                                                                                                                          |
| Device revision                            | <ul style="list-style-type: none"> <li>6 - SW version 03.00.zz</li> <li>7 - SW version 04.00.zz (FF-912)</li> </ul>                                                                                                                                                               |
| DD revision                                | <ul style="list-style-type: none"> <li>3 (device revision 6)</li> <li>2 (device revision 7)</li> </ul>                                                                                                                                                                            |
| CFF revision                               | <ul style="list-style-type: none"> <li>4 (device revision 6)</li> <li>1 (device revision 7)</li> </ul>                                                                                                                                                                            |
| DD files                                   | Information and files under:                                                                                                                                                                                                                                                      |
| CFF files                                  | <ul style="list-style-type: none"> <li><a href="http://www.endress.com">www.endress.com</a></li> <li><a href="http://www.fieldcommgroup.org">www.fieldcommgroup.org</a></li> </ul>                                                                                                |
| Device tester version (ITK version)        | <ul style="list-style-type: none"> <li>5.0 (device revision 6)</li> <li>6.01 (device revision 7)</li> </ul>                                                                                                                                                                       |
| Number of ITK test campaign                | <ul style="list-style-type: none"> <li>IT054600 (Device Revision 6)</li> <li>IT085500 (Device Revision 7)</li> </ul>                                                                                                                                                              |
| Link-Master (LAS) capable                  | Yes                                                                                                                                                                                                                                                                               |
| Choice of "Link Master" and "Basic Device" | Yes; Factory setting: Basic Device                                                                                                                                                                                                                                                |
| Node address                               | Factory setting: 247 (F7 hex)                                                                                                                                                                                                                                                     |
| Supported functions                        | <p>Field diagnostics profile (only with FF912)</p> <p>The following methods are supported:</p> <ul style="list-style-type: none"> <li>Reboot</li> <li>Configure error as warning or alarm</li> <li>HistoROM</li> <li>Peakhold</li> <li>Alarm info</li> <li>Sensor trim</li> </ul> |
| Number of VCRs                             | <ul style="list-style-type: none"> <li>44 (device revision 6)</li> <li>24 (device revision 7)</li> </ul>                                                                                                                                                                          |
| Number of Link Objects in VFD              | 50                                                                                                                                                                                                                                                                                |

### Virtual communication references (VCRs)

|                   | Device revision 6 | Device revision 7 |
|-------------------|-------------------|-------------------|
| Permanent Entries | 44                | 1                 |
| Client VCRs       | 0                 | 0                 |
| Server VCRs       | 5                 | 10                |
| Source VCRs       | 8                 | 43                |
| Sink VCRs         | 0                 | 0                 |
| Subscriber VCRs   | 12                | 43                |
| Publisher VCRs    | 19                | 43                |

### Link settings

|                      | Device revision 6 | Device revision 7 |
|----------------------|-------------------|-------------------|
| Slot time            | 4                 | 4                 |
| Min. Inter PDU delay | 12                | 10                |
| Max. response delay  | 10                | 10                |

### Transducer Blocks

| Block            | Contents                                            | Output values                                                                                                                                                                                             |
|------------------|-----------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| TRD1 Block       | Contains all parameters related to the measurement  | <ul style="list-style-type: none"> <li>■ Pressure or level (channel 1)</li> <li>■ Process temperature (channel 2)</li> </ul>                                                                              |
| Service Block    | Contains service information                        | <ul style="list-style-type: none"> <li>■ Pressure after damping (channel 3)</li> <li>■ Pressure peakhold indicator (channel 4)</li> <li>■ Counter for max. pressure transgressions (channel 5)</li> </ul> |
| Diagnostic block | Contains diagnostic information                     | Error code via DI channels (channel 0 to 16)                                                                                                                                                              |
| Display block    | Contains parameters to configure the onsite display | No output values                                                                                                                                                                                          |

### Function blocks

| Block                                        | Contents                                                                                                                                                                                                                                                                                                                                                                                                  | Number Blocks | Execution time    |                                         | Functionality     |                   |
|----------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------|-------------------|-----------------------------------------|-------------------|-------------------|
|                                              |                                                                                                                                                                                                                                                                                                                                                                                                           |               | Device Revision 6 | Device Revision 7                       | Device Revision 6 | Device Revision 7 |
| Resource Block                               | The Resource Block contains all the data that uniquely identify the device. It is an electronic version of a nameplate of the device.                                                                                                                                                                                                                                                                     | 1             |                   |                                         | enhanced          | enhanced          |
| Analog Input Block 1<br>Analog Input Block 2 | The AI Block receives the measuring data from the Sensor Block, (selectable via a channel number) and makes the data available to other function blocks at its output. Enhancement: Digital outputs for process alarms, fail safe mode                                                                                                                                                                    | 2             | 45 ms             | 45 ms (without trend and alarm reports) | enhanced          | enhanced          |
| Digital Input Block                          | This block contains the discrete data of the Diagnose Block (selectable via a channel number 0 to 16) and provides them for other blocks at the output.                                                                                                                                                                                                                                                   | 1             | 40 ms             | 30 ms                                   | standard          | enhanced          |
| Digital Output Block                         | This block converts the discrete input and thus initiates an action (selectable via a channel number) in the DP Flow Block or in the Service Block. Channel 1 resets the counter for max. pressure transgressions.                                                                                                                                                                                        | 1             | 60 ms             | 40 ms                                   | standard          | enhanced          |
| PID Block                                    | This block is used as a proportional-integral-derivative controller and can be used universally for closed-loop-control in the field. It enables cascade mode and feedforward control. Input IN can be indicated on the display. The selection is performed in the Display Block (DISPLAY_MAIN_LINE_CONTENT).                                                                                             | 1             | 120 ms            | 70 ms                                   | standard          | enhanced          |
| Arithmetic Block                             | This block is designed to permit simple use of popular measurement math functions. The user does not have to know how to write equations. The math algorithm is selected by name, chosen by the user for the function to be performed.                                                                                                                                                                    | 1             | 50 ms             | 40 ms                                   | standard          | enhanced          |
| Input Selector Block                         | The Input Selector Block facilitates the selection of up to four inputs and generates an output based on the configured action. This block normally receives its inputs from AI Blocks. The block enables the selection of maximum, minimum, average and 'first good' values. Inputs IN1 to IN4 can be shown on the display. The selection is performed in the Display Block (DISPLAY_MAIN_LINE_CONTENT). | 1             | 35 ms             | 35 ms                                   | standard          | enhanced          |
| Signal Characterizer Block                   | The Signal Characterizer Block has two sections, each with an output value that is a non-linear function of the input value. The non-linear function is generated by a single look-up table with 21 arbitrary x-y pairs.                                                                                                                                                                                  | 1             | 30 ms             | 40 ms                                   | standard          | enhanced          |
| Integrator Block                             | The Integrator Block integrates a variable as a function of the time or accumulates the counts from a Pulse Input Block. The block may be used as a totalizer that counts up until reset or as a batch totalizer that has a setpoint, where the integrated or accumulated value is compared to pre-trip and trip settings, generating a binary signal when the setpoint is reached.                       | 1             | 35 ms             | 40 ms                                   | standard          | enhanced          |
| Analog Alarm Block                           | This block contains all process alarm conditions (working like a comparator) and represents them at the output.                                                                                                                                                                                                                                                                                           | 1             | 35 ms             | 35 ms                                   | standard          | enhanced          |

### Additional function block information:

|                                                     |    |    |
|-----------------------------------------------------|----|----|
| Instantiate Function Block                          | JA | JA |
| Number of additional instantiatable function blocks | 11 | 5  |

## Energy supply


### **⚠ WARNING**

#### **An incorrect connection compromises electrical safety!**

- ▶ When using the measuring instrument in hazardous areas, installation must also comply with the applicable national standards and regulations and the Safety Instructions or Installation or Control Drawings.
- ▶ All explosion protection data are provided in separate Ex documentation, which is available on request. The Ex documentation is supplied as standard with all devices approved for use in explosion hazardous areas.
- ▶ Devices with integrated overvoltage protection must be grounded → 26.
- ▶ Protective circuits against reverse polarity, HF influences and overvoltage peaks are installed.

### Terminal assignment


#### 4 to 20 mA HART

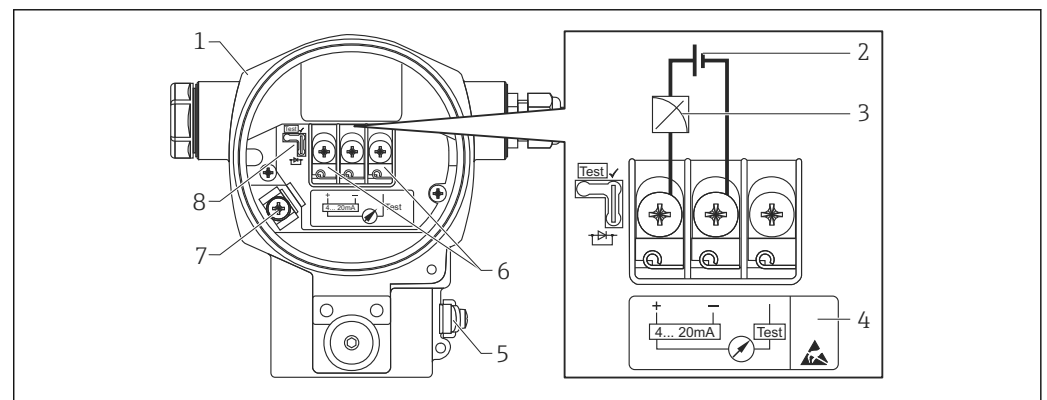

A0019989

- 1 Housing
- 2 Supply voltage
- 3 4 to 20 mA
- 4 Devices with integrated overvoltage protection are labeled "OVP" (overvoltage protection) here.
- 5 External ground terminal
- 6 4 to 20 mA test signal between positive and test terminal
- 7 Internal ground terminal
- 8 Jumper for 4 to 20 mA test signal → 22


#### 1-5V DC

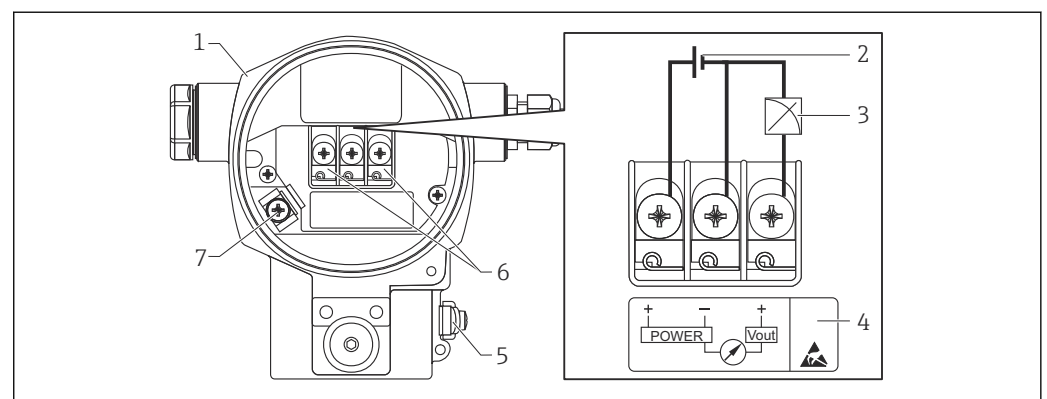

A0031676

- 1 Housing
- 2 Supply voltage
- 3 1-5V DC
- 4 Overvoltage protection (OVP) marking
- 5 External ground terminal
- 6 Terminals
- 7 Internal ground terminal

## PROFIBUS PA and FOUNDATION Fieldbus

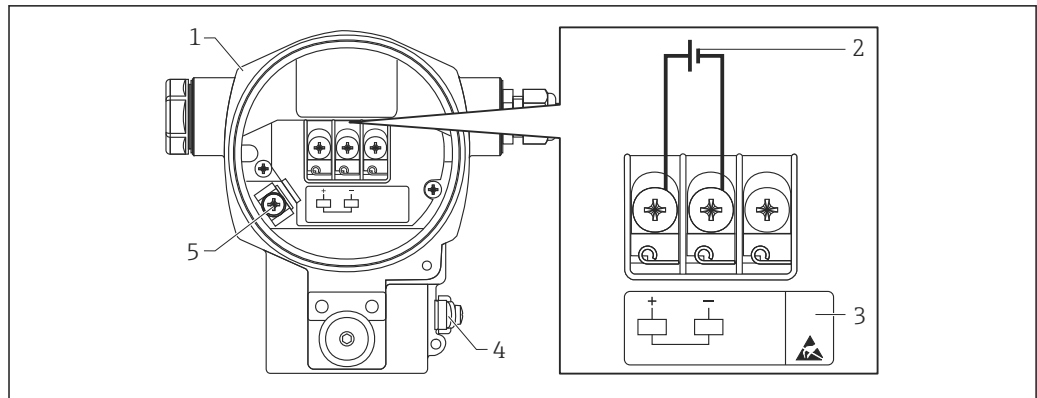

A0020158

- 1 Housing
- 2 Supply voltage
- 3 Devices with integrated overvoltage protection are labeled "OVP" (overvoltage protection) here.
- 4 External ground terminal
- 5 Internal ground terminal

## Supply voltage

### 4 to 20 mA HART

| Electronic version                                                                                                 | Jumper for 4 to 20 mA test signal in "Test" position (delivery status) | Jumper for 4 to 20 mA test signal in "Non-test" position     |
|--------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------|--------------------------------------------------------------|
| Version for non-hazardous area                                                                                     | 11.5 to 45 V DC                                                        | 10.5 to 45 V DC                                              |
| Intrinsically safe                                                                                                 | 11.5 to 30 V DC                                                        | 10.5 to 30 V DC                                              |
| <ul style="list-style-type: none"> <li>Other types of protection</li> <li>Devices without a certificate</li> </ul> | 11.5 to 45 V DC<br>(Versions with 35 V DC plug-in connector)           | 10.5 to 45 V DC<br>(Versions with 35 V DC plug-in connector) |

### Measuring a 4 to 20 mA test signal

| Jumper position for test signal | Description                                                                                                                                                                                                                                                                                 |
|---------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <p>A0019992</p>                 | <ul style="list-style-type: none"> <li>Measurement of 4 to 20 mA test signal via the positive and test terminal: possible. (Thus, the output current can be measured without interruption via the diode.)</li> <li>As-delivered state</li> <li>Minimum supply voltage: 11.5 V DC</li> </ul> |
| <p>A0019993</p>                 | <ul style="list-style-type: none"> <li>Measurement of 4 to 20 mA test signal via the positive and test terminal: not possible.</li> <li>Minimum supply voltage: 10.5 V DC</li> </ul>                                                                                                        |

### 1-5V DC

- Non-hazardous area: 9 to 35 V DC
- Ex-d: 9 to 35 V DC

**PROFIBUS PA**

- Version for non-hazardous areas: 9 to 32 V DC
- Ex ia:
  - Installation in bus system according to FISCO model:  $U_i=17.5$  V DC
  - Point-to-point installation:  $U_i = 24$  V DC

**FOUNDATION Fieldbus**

- Version for non-hazardous areas: 9 to 32 V DC
- Ex ia:
  - Installation in bus system according to FISCO model:  $U_i=17.5$  V DC
  - Point-to-point installation:  $U_i = 24$  V DC

**Current consumption**

- 1-5V DC:
  - 9 V = 1.8 mA
  - 35 V = 0.8 mA
- PROFIBUS PA: 13 mA  $\pm$  1 mA, switch-on current corresponds to IEC 61158-2, Clause 21
- FOUNDATION Fieldbus: 15.5 mA  $\pm$  1 mA, switch-on current corresponds to IEC 61158-2, Clause 21

**Electrical connection****PROFIBUS PA**

The digital communication signal is transmitted to the bus via a two-wire connection. The bus also provides the power supply. For further information on the network structure and grounding and for further bus system components such as bus cables, see the relevant documentation, e.g. Operating Instructions BA00034S "PROFIBUS DP/PA: Guidelines for planning and commissioning" and the PNO Guideline.

**FOUNDATION Fieldbus**

The digital communication signal is transmitted to the bus via a two-wire connection. The bus also provides the power supply. For further information on the network structure and grounding and for further bus system components such as bus cables, see the relevant documentation, e.g. Operating Instructions BA00013S "FOUNDATION Fieldbus Overview" and the FOUNDATION Fieldbus Guideline.

**Terminals**

- Supply voltage and internal ground terminal: 0.5 to 2.5 mm<sup>2</sup> (20 to 14 AWG)
- External ground terminal: 0.5 to 4 mm<sup>2</sup> (20 to 12 AWG)

**Cable entries**

| Approval                                                              | Cable gland          | Clamping range                 |
|-----------------------------------------------------------------------|----------------------|--------------------------------|
| Standard, II 1/2 G Ex ia, IS                                          | Plastic M20x1.5      | 5 to 10 mm (0.2 to 0.39 in)    |
| ATEX II 1/2 D, II 1/3 D, II 1/2 GD Ex ia, II 1 GD Ex ia, II 3 G Ex nA | Metal M20x1.5 (Ex e) | 7 to 10.5 mm (0.28 to 0.41 in) |


**1-5V DC**

The cable entries have a 1/2 FNPT thread. The connection on the customer's side is protected by a plastic connector. A cable gland is not envisaged.

For additional technical data, see section on housing →  51

## Connectors

### Connection of devices with Harting plug Han7D

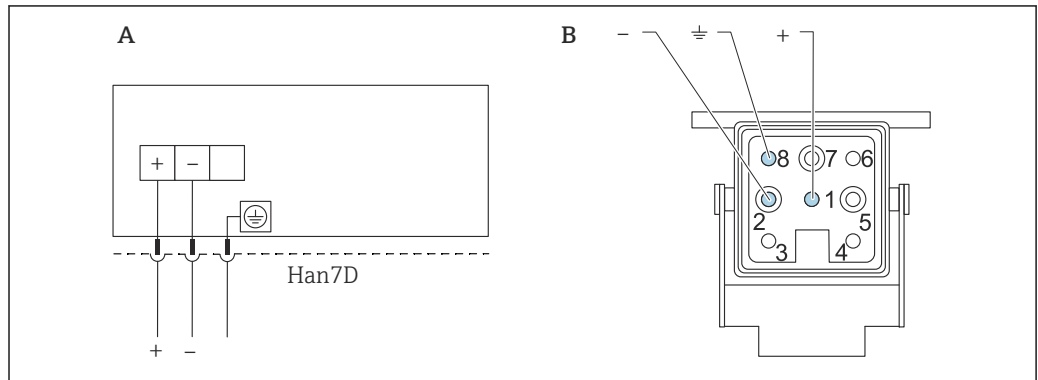

A0019990

A Electrical connection for devices with Harting plug Han7D

B View of the connection on the device


- Brown

≡ Green/yellow

+ Blue

Material: CuZn, gold-plated contacts of the plug-in jack and plug

### Connection of cable version

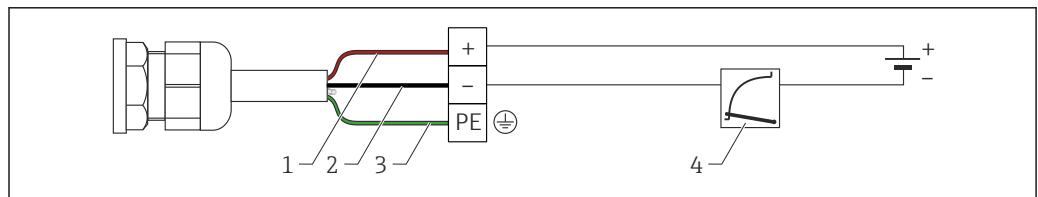

A0019991


1 rd = red

2 bk = black

3 gnye = green

4 4 to 20 mA

### Connection of cable version 1-5V DC

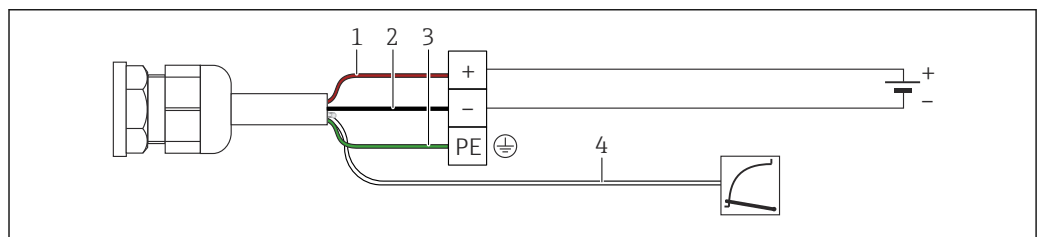

A0032269


1 rd = red

2 bk = black

3 gnye = green

4 1-5V DC

### Connection of devices with M12 plug

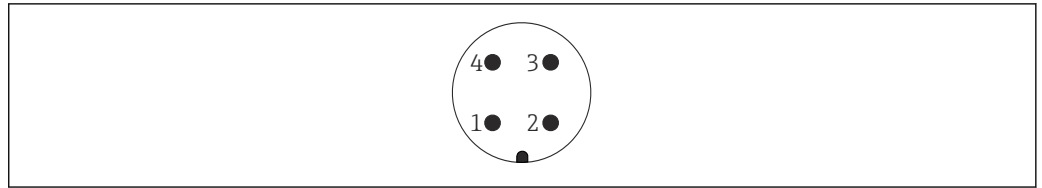

A0011175

- 1 *Signal +*
- 2 *Not used*
- 3 *Signal -*
- 4 *Ground*

Endress+Hauser offers the following accessories for devices with an M12 plug:

Plug-in jack M 12x1, straight

- Material: body PA; coupling nut CuZn, nickel-plated
- Degree of protection (fully locked): IP67
- Order number: 52006263


Plug-in jack M 12x1, elbowed

- Material: body PBT/PA; coupling nut GD-Zn, nickel-plated
- Degree of protection (fully locked): IP67
- Order number: 71114212

Cable 4x0.34 mm<sup>2</sup> (20 AWG) with M12 elbowed socket, screw plug, length 5 m (16 ft)

- Material: body PUR; coupling nut CuSn/Ni; cable PVC
- Degree of protection (fully locked): IP67
- Order number: 52010285

### Connection of devices with 7/8" plug

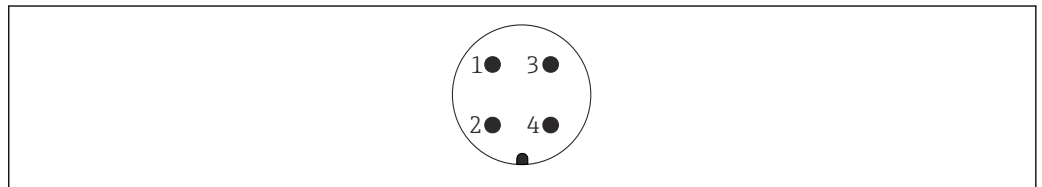

A0011176

- 1 *Signal -*
- 2 *Signal +*
- 3 *Shield*
- 4 *Not used*

Male thread: 7/8 - 16 UNC

- Material: 316L (1.4401)
- Degree of protection: IP68

### Cable specification

#### HART

- Endress+Hauser recommends using shielded, twisted-pair two-wire cables.
- Cable outer diameter: 5 to 9 mm (0.2 to 0.35 in) depending on the cable entry used →  23

#### 1-5V DC

- Endress+Hauser recommends using a shielded cable.
- Cable outer diameter: 5 to 9 mm (0.2 to 0.35 in) depending on the cable entry used →  23

*Maximum cable length*

The following table shows the tolerance of the voltage output for a representative cable with a length of up to 100 m (328 ft), a resistance of 18 Ohm/km and specification 18 AWG (cable cross-section 0.8 mm<sup>2</sup>).

| Tolerance of voltage output at cable end | Length         |
|------------------------------------------|----------------|
| 0.5 mV                                   | 25 m (82 ft)   |
| 1 mV                                     | 50 m (164 ft)  |
| 1.5 mV                                   | 75 m (246 ft)  |
| 2 mV                                     | 100 m (328 ft) |

**PROFIBUS PA**

Use a twisted, shielded twin-core cable, preferably cable type A.



For further information on the cable specifications, see Operating Instructions BA00034S "PROFIBUS DP/PA: Guidelines for planning and commissioning", the PNO Guideline 2.092 PROFIBUS PA User and Installation Guideline" and IEC 61158-2 (MBP).

**FOUNDATION Fieldbus**

Use a twisted, shielded twin-core cable, preferably cable type A.



For further information on the cable specifications, see Operating Instructions BA00013S "FOUNDATION Fieldbus Overview", FOUNDATION Fieldbus Guideline and IEC 61158-2 (MBP).

|                                                                                          |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
|------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Start-up current</b>                                                                  | 12 mA                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |
| <b>Residual ripple</b>                                                                   | Without influence on 4 to 20 mA signal up to $\pm 5\%$ residual ripple within the permitted voltage range [according to HART hardware specification HCF_SPEC-54 (DIN IEC 60381-1)].                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>Overvoltage protection (optionally for HART, PROFIBUS PA and FOUNDATION Fieldbus)</b> | <ul style="list-style-type: none"> <li>■ Overvoltage protection: <ul style="list-style-type: none"> <li>■ Nominal functioning DC voltage: 600 V</li> <li>■ Nominal discharge current: 10 kA</li> </ul> </li> <li>■ Surge current check <math>\hat{i} = 20</math> kA satisfied as per DIN EN 60079-14: 8/20 <math>\mu</math>s</li> <li>■ Arrester AC current check <math>I = 10</math> A satisfied</li> </ul> <p>Ordering information: Product Configurator, order code for "Additional options 1" or Additional options 2", option "M"</p> <p><b>NOTICE</b></p> <p><b>Device could be destroyed!</b></p> <p>► Devices with integrated overvoltage protection must be grounded.</p> |
| <b>Influence of power supply</b>                                                         | $\leq 0.0006$ % of URL/1 V                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         |

## Performance characteristics for measuring instruments with ceramic process membrane

|                                       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
|---------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Response time</b>                  | <p><b>HART</b></p> <ul style="list-style-type: none"> <li>■ Acyclic: min. 330 ms, typically 590 ms (depending on command # and number of preambles)</li> <li>■ Cyclic (burst): min. 160 ms, typically 350 ms (depending on command # and number of preambles)</li> </ul> <p><b>PROFIBUS PA</b></p> <ul style="list-style-type: none"> <li>■ Acyclic: approx. 60 ms to 70 ms (depending on Min. Slave Interval)</li> <li>■ Cyclic: approx. 10 ms to 13 ms (depending on Min. Slave Interval)</li> </ul> <p><b>FOUNDATION Fieldbus</b></p> <ul style="list-style-type: none"> <li>■ Acyclic: typically 100 ms (for standard bus parameter settings)</li> <li>■ Cyclic: max. 20 ms (for standard bus parameter settings)</li> </ul>                                                                                                                                                                                                                                       |
| <b>Reference operating conditions</b> | <ul style="list-style-type: none"> <li>■ As per IEC 62828-2 / IEC 60770</li> <li>■ Ambient temperature <math>T_A</math> = constant, in the range: +22 to +28 °C (+72 to +82 °F)</li> <li>■ Humidity <math>\phi</math> = constant, in the range: 5 to 80 % RH <math>\pm</math> 5 %</li> <li>■ Atmospheric pressure <math>p_A</math> = constant, in the range: 860 to 1 060 mbar (12.47 to 15.37 psi)</li> <li>■ Position of the measuring cell: horizontal <math>\pm</math>1°</li> <li>■ Input of LOW SENSOR TRIM and HIGH SENSOR TRIM for lower range value and upper range value</li> <li>■ Zero-point based span</li> <li>■ Process membrane material: Al<sub>2</sub>O<sub>3</sub> aluminum oxide ceramic FDA, ultrapure 99.9 %</li> <li>■ Supply voltage: 24 V DC <math>\pm</math>3 V DC</li> <li>■ Load with HART: 250 <math>\Omega</math></li> <li>■ Turn down (TD) = URL/   URV - LRV  </li> </ul>                                                               |
| <b>Total performance</b>              | <p>The performance characteristics refer to the accuracy of the device. The factors that influence the accuracy can be divided into two groups</p> <ul style="list-style-type: none"> <li>■ Total performance of device</li> <li>■ Installation factors</li> </ul> <p>All of the performance characteristics meet the requirement of <math>\geq \pm 3</math> sigma.</p> <p>The total performance of the device comprises the reference accuracy and the ambient temperature effect and is calculated using the following formula:</p> $\text{Total performance} = \pm \sqrt{(E1)^2 + (E2)^2}$ <p>E1 = Reference accuracy<br/>E2 = Temperature effect</p> <p>Calculation of E2:</p> <p>Temperature effect per <math>\pm 28</math> °C (50 °F)<br/>(Corresponds to a range of -3 to +53 °C (+27 to +127 °F))</p> $E2 = E2_M + E2_E$ <p>E2<sub>M</sub> = Main temperature error<br/>E2<sub>E</sub> = Electronics error</p> <p>The values refer to the calibrated span.</p> |

**Calculation of the total performance with the Endress+Hauser Applicator**

Detailed inaccuracies, e.g. for other temperature ranges or the high-temperature version of the device can be calculated with the Applicator "[Sizing Pressure Performance](#)".



A0038927

**Reference accuracy [E1]**

Reference accuracy comprises the non-linearity [IEC 62828-1/DIN EN 61298-2] including the hysteresis [IEC 62828-1/DIN EN 61298-2] and the non-repeatability [IEC 62828-1/DIN EN 61298-2] in accordance with the limit point method as per [IEC 62828-1/DIN EN 60770-2]. Reference accuracy for standard up to TD 100:1, for platinum up to TD 5:1.

100 mbar (1.5 psi) measuring cell

- Standard:  $TD \leq 10:1 = \pm 0.075 \%$ ;  $TD > 10:1 = \pm 0.0075 \% \cdot TD$
- Platinum:  $TD 1:1 = \pm 0.05 \%$ ;  $TD > 1:1 = \pm 0.075 \%$

250 mbar (3.75 psi) measuring cell

- Standard:  $TD \leq 10:1 = \pm 0.075 \%$ ;  $TD > 10:1 = \pm 0.0075 \% \cdot TD$
- Platinum:  $TD \geq 1:1 = \pm 0.05 \%$

400 mbar (6 psi) and 1 bar (15 psi) measuring cell

- Standard:  $TD \leq 10:1 = \pm 0.05 \%$ ;  $TD > 10:1 = \pm 0.005 \% \cdot TD$
- Platinum:  $TD \geq 1:1 = \pm 0.035 \%$

2 bar (30 psi) measuring cell

- Standard:  $TD \leq 10:1 = \pm 0.05 \%$ ;  $TD > 10:1 = \pm 0.005 \% \cdot TD$
- Platinum:  $TD 1:1 = \pm 0.025 \%$ ;  $TD \geq 1:1 = \pm 0.035 \%$

4 bar (60 psi) measuring cell

- Standard:  $TD \leq 10:1 = \pm 0.05 \%$ ;  $TD > 10:1 = \pm 0.005 \% \cdot TD$
- Platinum:  $TD \geq 1:1 = \pm 0.025 \%$

10 bar (150 psi) and 40 bar (600 psi) measuring cell

- Standard:  $TD \leq 10:1 = \pm 0.05 \%$ ;  $TD > 10:1 = \pm 0.005 \% \cdot TD$
- Platinum:  $TD \geq 1:1 = \pm 0.035 \%$

**Measuring uncertainty for small absolute pressure measuring ranges**

The smallest extended uncertainty of measurement that can be delivered by our standards in the 0.001 to 35 mbar (0.0000145 to 0.5075 psi) range is 0.1 % of the reading + 0.004 mbar (0.000058 psi).

Temperature effect [E2]

$E2_M$  - Main temperature error

The output changes due to the effect of the ambient temperature [IEC 62828-1/IEC 61298-3] with respect to the reference temperature [IEC 62828-1/DIN 16086]. The values specify the maximum error due to min./max. ambient or process temperature conditions.

100 mbar (1.5 psi), 250 mbar (3.75 psi) and 400 mbar (6 psi) measuring cell

- Standard:  $\pm (0.07 \% \cdot TD + 0.038 \%)$
- Platinum:  $\pm (0.07 \% \cdot TD + 0.038 \%)$

1 bar (15 psi), 2 bar (30 psi), 4 bar (60 psi), 10 bar (150 psi) and 40 bar (600 psi) measuring cell

- Standard:  $\pm (0.065 \% \cdot TD + 0.02 \%)$
- Platinum:  $\pm (0.065 \% \cdot TD + 0.02 \%)$

$E2_E$  - Electronics error

- Analog output (4 to 20 mA): 0.05 %
- Digital output (HART/PA/FF): 0 %

**Resolution** Current output: 1  $\mu$ A

**Total error** The total error of the device comprises the total performance and the long-term stability effect and is calculated using the following formula:  
Total error = total performance + long-term stability

Calculation of the total error with the Endress+Hauser Applicator

Detailed inaccuracies, e.g. for other temperature ranges or the high-temperature version of the device can be calculated with the Applicator "[Sizing Pressure Performance](#)".



A0038927

Calculation of the diaphragm seal error with the Endress+Hauser Applicator

Diaphragm seal errors are not taken into consideration. They are calculated separately in the Applicator "[Sizing Diaphragm Seal](#)".



A0038925

**Long-term stability** The specifications refer to the upper range limit (URL).

Gauge pressure measuring cells

- 1 year:  $\pm 0.05\%$
- 5 years:  $\pm 0.08\%$
- 10 years:  $\pm 0.10\%$


Absolute pressure measuring cells

- 1 year:  $\pm 0.05\%$
- 5 years:  $\pm 0.15\%$
- 10 years:  $\pm 0.20\%$

## Response time T63 and T90

### Dead time, time constant

Representation of dead time and time constant as per IEC62828-1:

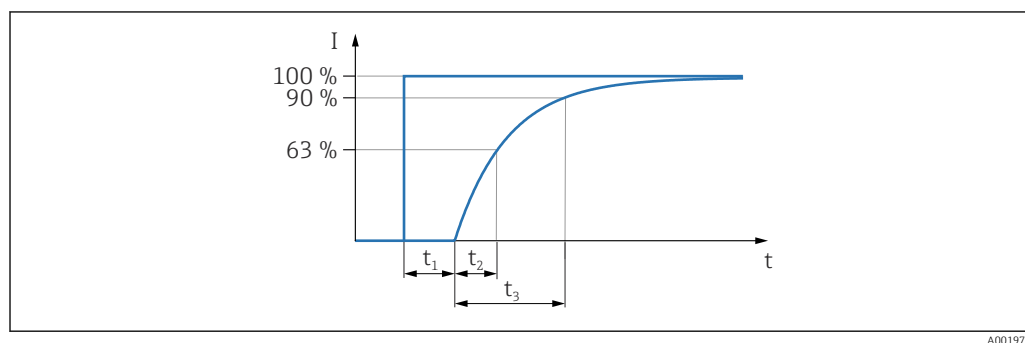

A0019786

Step response time = dead time ( $t_1$ ) + time constant T90 ( $t_3$ ) according to IEC62828-1

### Dynamic behavior, current output

|      | Dead time ( $t_1$ ) | Time constant T63 ( $t_2$ ) | Time constant T90 ( $t_3$ ) |
|------|---------------------|-----------------------------|-----------------------------|
| Max. | 90 ms               | 120 ms                      | 276 ms                      |

### Dynamic behavior, digital output (HART electronics)

A typical burst rate of 300 ms results in the following behavior:

|      | Dead time ( $t_1$ ) | Dead time ( $t_1$ ) + Time constant T63 ( $t_2$ ) | Dead time ( $t_1$ ) + Time constant T90 ( $t_3$ ) |
|------|---------------------|---------------------------------------------------|---------------------------------------------------|
| Min. | 250 ms              | 370 ms                                            | 436 ms                                            |
| Max. | 1050 ms             | 1170 ms                                           | 1236 ms                                           |

### Read cycle

- Acyclic: max. 3/s, typically 1/s (depends on command # and number of preambles)
- Cyclic (burst): max. 3/s, typically 2/s

The device commands the BURST MODE function for cyclic value transmission via the HART communication protocol.

### Cycle time (update time)

Cyclic (burst): min. 300 ms

### Dynamic behavior, PROFIBUS PA

A typical PLC cycle time of 1 s results in the following behavior:

|      | Dead time ( $t_1$ ) | Dead time ( $t_1$ ) + Time constant T63 ( $t_2$ ) | Dead time ( $t_1$ ) + Time constant T90 ( $t_3$ ) |
|------|---------------------|---------------------------------------------------|---------------------------------------------------|
| Min. | 125 ms              | 245 ms                                            | 311 ms                                            |
| Max. | 1325 ms             | 1445 ms                                           | 1511 ms                                           |

#### Read cycle (PLC)

- Acyclic: typically 25/s
- Cyclic: typically 30/s (depending on the number and type of function blocks used in the closed-control loop)

#### Cycle time (update time)

Min. 200 ms

The cycle time in a bus segment in cyclic data communication depends on the number of devices, on the segment coupler used and on the internal PLC cycle time. A new measured value can be determined up to five times a second.

#### Dynamic behavior, FOUNDATION Fieldbus

A typical configuration for the macro cycle time (host system) of 1 s results in the following behavior:

|      | Dead time ( $t_1$ ) | Dead time ( $t_1$ ) +<br>Time constant T63 ( $t_2$ ) | Dead time ( $t_1$ ) +<br>Time constant T90 ( $t_3$ ) |
|------|---------------------|------------------------------------------------------|------------------------------------------------------|
| Min. | 135 ms              | 255 ms                                               | 321 ms                                               |
| Max. | 1135 ms             | 1255 ms                                              | 1321 ms                                              |

#### Read cycle

- Acyclic: typically 10/s
- Cyclic: max. 10/s (depending on the number and type of function blocks used in a closed-control loop)

#### Cycle time (update time)

Cyclic: min. 100 ms

#### Installation factors

##### Influence of installation position

≤ 0.18 mbar (0.003 psi). Device rotated 180°, process connection pointing upwards.

 A position-dependent zero point shift can be corrected. Please refer to the "Commissioning → Position adjustment" section of the Operating Instructions.

Different tightening torques (e.g. for Clamp or Varivent connections) can merely cause a shift in the zero point. This effect is corrected by position adjustment during commissioning.

##### Warm-up period

- 4 to 20 mA HART: < 10 s
- PROFIBUS PA: 6 s
- FOUNDATION Fieldbus: 50 s

## Performance characteristics for measuring instruments with metallic process membrane

|                                       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
|---------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Response time</b>                  | <p><b>HART</b></p> <ul style="list-style-type: none"> <li>■ Acyclic: min. 330 ms, typically 590 ms (depending on command # and number of preambles)</li> <li>■ Cyclic (burst): min. 160 ms, typically 350 ms (depending on command # and number of preambles)</li> </ul> <p><b>PROFIBUS PA</b></p> <ul style="list-style-type: none"> <li>■ Acyclic: approx. 60 ms to 70 ms (depending on Min. Slave Interval)</li> <li>■ Cyclic: approx. 10 ms to 13 ms (depending on Min. Slave Interval)</li> </ul> <p><b>FOUNDATION Fieldbus</b></p> <ul style="list-style-type: none"> <li>■ Acyclic: typically 100 ms (for standard bus parameter settings)</li> <li>■ Cyclic: max. 20 ms (for standard bus parameter settings)</li> </ul>                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
| <b>Reference operating conditions</b> | <ul style="list-style-type: none"> <li>■ As per IEC 62828-2 / IEC 60770</li> <li>■ Ambient temperature <math>T_A</math> = constant, in the range: +22 to +28 °C (+72 to +82 °F)</li> <li>■ Humidity <math>\phi</math> = constant, in the range: 5 to 80 % RH <math>\pm</math> 5 %</li> <li>■ Atmospheric pressure <math>p_A</math> = constant, in the range: 860 to 1 060 mbar (12.47 to 15.37 psi)</li> <li>■ Position of the measuring cell: horizontal <math>\pm</math> 1°</li> <li>■ Input of LOW SENSOR TRIM and HIGH SENSOR TRIM for lower range value and upper range value</li> <li>■ Zero-point based span</li> <li>■ Process membrane material: AISI 316L (1.4435) or Alloy C</li> <li>■ Fill fluid PMP71/PMP75: silicone oil</li> <li>■ Supply voltage: 24 V DC <math>\pm</math> 3 V DC</li> <li>■ Load with HART: 250 <math>\Omega</math></li> <li>■ Turn down (TD) = URL/   URV - LRV  </li> </ul>                                                                                                                                                                                                                                                                                                      |
| <b>Total performance</b>              | <p>The performance characteristics refer to the accuracy of the device. The factors that influence the accuracy can be divided into two groups</p> <ul style="list-style-type: none"> <li>■ Total performance of device</li> <li>■ Installation factors</li> </ul> <p>All of the performance characteristics meet the requirement of <math>\geq \pm 3</math> sigma.</p> <p>The total performance of the device comprises the reference accuracy and the ambient temperature effect and is calculated using the following formula:</p> $\text{Total performance} = \pm \sqrt{(E1)^2 + (E2)^2}$ <p><math>E1</math> = Reference accuracy</p> <p><math>E2</math> = Ambient temperature effect</p> <p>Calculation of <math>E2</math>:</p> <p>Ambient temperature effect per <math>\pm 28</math> °C (50 °F)</p> <p>(Corresponds to a range of <math>-3</math> to <math>+53</math> °C (<math>+27</math> to <math>+127</math> °F))</p> $E2 = E2_M + E2_E$ <p><math>E2_M</math> = Main temperature error</p> <p><math>E2_E</math> = Electronics error</p> <ul style="list-style-type: none"> <li>■ The values apply to process membranes made of 316L (1.4435)</li> <li>■ The values refer to the calibrated span.</li> </ul> |

### Calculation of the total performance with the Endress+Hauser Applicator

Detailed inaccuracies, e.g. for other temperature ranges, can be calculated with the Applicator ["Sizing Pressure Performance"](#).



A0038927

### Calculation of the diaphragm seal error with the Endress+Hauser Applicator

Diaphragm seal errors are not taken into consideration. They are calculated separately in the Applicator ["Sizing Diaphragm Seal"](#).



A0038925

**Reference accuracy [E1]**

Reference accuracy comprises the non-linearity [IEC 62828-1/DIN EN 61298-2] including the hysteresis [IEC 62828-1/DIN EN 61298-2] and the non-repeatability [IEC 62828-1/DIN EN 61298-2] in accordance with the limit point method as per [IEC 62828-1/DIN EN 60770-2]. Reference accuracy for standard up to TD 100:1, for platinum up to TD 5:1.

*PMP71*

400 mbar (6 psi) measuring cell

- Standard: TD 1:1 =  $\pm 0.05\%$ ; TD > 1:1 =  $\pm 0.05\% \cdot \text{TD}$
- Platinum: TD 1:1 =  $\pm 0.025\%$ ; TD > 1:1 =  $\pm 0.04\%$

1 bar (15 psi) measuring cell

- Standard: TD  $\leq 2.5:1$  =  $\pm 0.05\%$ ; TD > 2.5:1 =  $\pm 0.02\% \cdot \text{TD}$
- Platinum: TD 1:1 =  $\pm 0.025\%$ ; TD > 1:1 =  $\pm 0.03\%$

2 bar (30 psi) measuring cell

- Standard: TD  $\leq 5:1$  =  $\pm 0.05\%$ ; TD > 5:1 =  $\pm 0.01\% \cdot \text{TD}$
- Platinum: TD 1:1 =  $\pm 0.025\%$ ; TD > 1:1 =  $\pm 0.03\%$

4 bar (60 psi), 10 bar (150 psi) and 40 bar (600 psi) measuring cell

- Standard: TD  $\leq 10:1$  =  $\pm 0.05\%$ ; TD > 10:1 =  $\pm 0.005\% \cdot \text{TD}$
- Platinum: TD 1:1 =  $\pm 0.025\%$ ; TD > 1:1 =  $\pm 0.03\%$

100 bar (1 500 psi) measuring cell

- Standard: TD  $\leq 10:1$  =  $\pm 0.05\%$ ; TD > 10:1 =  $\pm 0.005\% \cdot \text{TD}$
- Platinum: TD 1:1 =  $\pm 0.035\%$ ; TD > 1:1 =  $\pm 0.04\%$

400 bar (6 000 psi) and 700 bar (10 500 psi) measuring cell

- Standard: TD  $\leq 5:1$  =  $\pm 0.1\%$ ; TD > 5:1 =  $\pm 0.02\% \cdot \text{TD}$
- Platinum: TD 1:1 =  $\pm 0.065\%$ ; TD > 1:1 =  $\pm 0.09\%$

PMP71 with 1-5V DC:

- 400 mbar (6 psi) to 100 bar (1 500 psi) measuring cell, multiply values by a factor of 2
- 400 bar (6 000 psi) and 700 bar (10 500 psi) measuring cell, multiply values by a factor of 1.5

Platinum not for flush-mounted process connections G ½ and M20.

*PMP75*

400 mbar (6 psi) measuring cell

Standard: TD 1:1 =  $\pm 0.15\%$ ; TD > 1:1 =  $\pm 0.15\% \cdot \text{TD}$

1 bar (15 psi) measuring cell

Standard: TD  $\leq 2.5:1$  =  $\pm 0.075\%$ ; TD > 2.5:1 =  $\pm 0.03\% \cdot \text{TD}$

2 bar (30 psi) measuring cell

Standard: TD  $\leq 5:1$  =  $\pm 0.075\%$ ; TD > 5:1 =  $\pm 0.015\% \cdot \text{TD}$

4 bar (60 psi), 10 bar (150 psi), 40 bar (600 psi) and 100 bar (1 500 psi) measuring cell

Standard: TD  $\leq 10:1$  =  $\pm 0.075\%$ ; TD > 10:1 =  $\pm 0.0075\% \cdot \text{TD}$

400 bar (6 000 psi) measuring cell

Standard: TD  $\leq 5:1$  =  $\pm 0.15\%$ ; TD > 5:1 =  $\pm 0.03\% \cdot \text{TD}$

**Measuring uncertainty for small absolute pressure measuring ranges**

The smallest extended uncertainty of measurement that can be delivered by our standards in the 0.001 to 35 mbar (0.0000145 to 0.5075 psi) range is 0.1 % of the reading + 0.004 mbar (0.000058 psi).

**Temperature effect [E2]**

*E2<sub>M</sub> - Main temperature error*

The output changes due to the effect of the ambient temperature [IEC 62828-1/IEC 61298-3] with respect to the reference temperature [IEC 62828-1/DIN 16086]. The values specify the maximum error due to min./max. ambient or process temperature conditions.

400 mbar (6 psi), 1 bar (15 psi), 2 bar (30 psi) and 4 bar (60 psi) measuring cell  
 $\pm (0.04 \% \cdot TD + 0.08 \%)$

10 bar (150 psi) and 40 bar (600 psi) measuring cell  
 $\pm (0.03 \% \cdot TD + 0.03 \%)$

100 bar (1 500 psi), 400 bar (6 000 psi) and 700 bar (10 500 psi) measuring cell  
 $\pm (0.015 \% \cdot TD + 0.06 \%)$

*E2<sub>E</sub> - Electronics error*

- Analog output (4 to 20 mA): 0.05 %
- Digital output (HART/PA/FF): 0 %
- PMP71 with 1-5V DC: 0.18 %

The additional electronics error that occurs in the temperature range -50 to -41 °C (-58 to -42 °F) is covered by E2<sub>LT</sub>.

*E2<sub>LT</sub> - low-temperature error*

The specifications refer to the calibrated span.

- -40 to +85 °C (-40 to +185 °F): 0 %
- -50 to -41 °C (-58 to -42 °F): 1.5 %

|                    |                                                                                                                                                                                                                     |
|--------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>Resolution</b>  | Current output: 1 µA                                                                                                                                                                                                |
|                    | Voltage output: 1 mW                                                                                                                                                                                                |
| <b>Total error</b> | <p>The total error of the device comprises the total performance and the long-term stability effect and is calculated using the following formula:</p> <p>Total error = total performance + long-term stability</p> |

**Calculation of the total error with the Endress+Hauser Applicator**

Detailed inaccuracies, e.g. for other temperature ranges, can be calculated with the Applicator ["Sizing Pressure Performance"](#).



A0038927

**Calculation of the diaphragm seal error with the Endress+Hauser Applicator**

Diaphragm seal errors are not taken into consideration. They are calculated separately in the Applicator ["Sizing Diaphragm Seal"](#).



A0038925

**Long-term stability**

The specifications refer to the upper range limit (URL).

2 bar (30 psi) measuring cell


- 1 year:  $\pm 0.07\%$
- 5 years:  $\pm 0.12\%$
- 10 years:  $\pm 0.15\%$

All other measuring cells

- 1 year:  $\pm 0.05\%$
- 5 years:  $\pm 0.07\%$
- 10 years:  $\pm 0.10\%$

**Response time T63 and T90****Dead time, time constant**

Representation of dead time and time constant as per IEC62828-1:

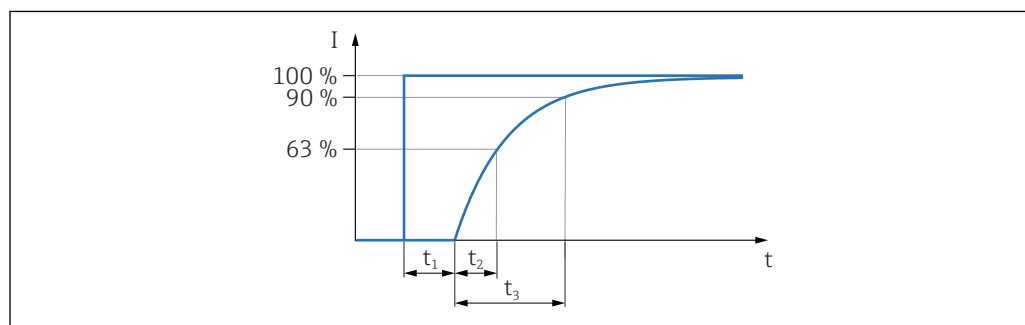

A0019786

Step response time = dead time ( $t_1$ ) + time constant T90 ( $t_3$ ) according to IEC62828-1

**Dynamic behavior, current output**

| Type  |      | Measuring cell                                                                                                   | Dead time ( $t_1$ ) | Time constant T63 ( $t_2$ )                                                | Time constant T90 ( $t_3$ )                                                 |
|-------|------|------------------------------------------------------------------------------------------------------------------|---------------------|----------------------------------------------------------------------------|-----------------------------------------------------------------------------|
| PMP71 | Max. | <ul style="list-style-type: none"> <li>■ 400 mbar (6 psi)</li> <li>■ <math>\geq 1</math> bar (15 psi)</li> </ul> | 45 ms               | <ul style="list-style-type: none"> <li>■ 70 ms</li> <li>■ 35 ms</li> </ul> | <ul style="list-style-type: none"> <li>■ 161 ms</li> <li>■ 81 ms</li> </ul> |
| PMP75 | Max. | PMP71 + influence of the diaphragm seal                                                                          |                     |                                                                            |                                                                             |

**Dynamic behavior, digital output (HART electronics)**

A typical burst rate of 300 ms results in the following behavior:

| Type  |      | Measuring cell                                                                                                   | Dead time ( $t_1$ ) | Dead time ( $t_1$ ) + Time constant T63 ( $t_2$ )                              | Dead time ( $t_1$ ) + Time constant T90 ( $t_3$ )                              |
|-------|------|------------------------------------------------------------------------------------------------------------------|---------------------|--------------------------------------------------------------------------------|--------------------------------------------------------------------------------|
| PMP71 | Min. | <ul style="list-style-type: none"> <li>■ 400 mbar (6 psi)</li> <li>■ <math>\geq 1</math> bar (15 psi)</li> </ul> | 205 ms              | <ul style="list-style-type: none"> <li>■ 275 ms</li> <li>■ 240 ms</li> </ul>   | <ul style="list-style-type: none"> <li>■ 321 ms</li> <li>■ 241 ms</li> </ul>   |
|       | Max. | <ul style="list-style-type: none"> <li>■ 400 mbar (6 psi)</li> <li>■ <math>\geq 1</math> bar (15 psi)</li> </ul> | 1005 ms             | <ul style="list-style-type: none"> <li>■ 1075 ms</li> <li>■ 1040 ms</li> </ul> | <ul style="list-style-type: none"> <li>■ 1121 ms</li> <li>■ 1041 ms</li> </ul> |
| PMP75 | Max. | PMP71 + influence of the diaphragm seal                                                                          |                     |                                                                                |                                                                                |

*Read cycle*

- Acyclic: max. 3/s, typically 1/s (depends on command # and number of preambles)
- Cyclic (burst): max. 3/s, typically 2/s

The device commands the BURST MODE function for cyclic value transmission via the HART communication protocol.

*Cycle time (update time)*

Cyclic (burst): min. 300 ms

**Dynamic behavior, 1-5V DC**

| Type  |      | Measuring cell | Dead time ( $t_1$ ) | Time constant T63 ( $t_2$ ) | Time constant T90 ( $t_3$ ) |
|-------|------|----------------|---------------------|-----------------------------|-----------------------------|
| PMP71 | Max. | All            | 40 ms               | 70 ms                       | 180 ms                      |

**Dynamic behavior, PROFIBUS PA**

A typical PLC cycle time of 1 s results in the following behavior:

| Type  |      | Measuring cell                                                                                                   | Dead time ( $t_1$ ) | Dead time ( $t_1$ ) + Time constant T63 ( $t_2$ )                              | Dead time ( $t_1$ ) + Time constant T90 ( $t_3$ )                              |
|-------|------|------------------------------------------------------------------------------------------------------------------|---------------------|--------------------------------------------------------------------------------|--------------------------------------------------------------------------------|
| PMP71 | Min. | <ul style="list-style-type: none"> <li>■ 400 mbar (6 psi)</li> <li>■ <math>\geq 1</math> bar (15 psi)</li> </ul> | 80 ms               | <ul style="list-style-type: none"> <li>■ 150 ms</li> <li>■ 115 ms</li> </ul>   | <ul style="list-style-type: none"> <li>■ 196 ms</li> <li>■ 116 ms</li> </ul>   |
|       | Max. | <ul style="list-style-type: none"> <li>■ 400 mbar (6 psi)</li> <li>■ <math>\geq 1</math> bar (15 psi)</li> </ul> | 1280 ms             | <ul style="list-style-type: none"> <li>■ 1350 ms</li> <li>■ 1315 ms</li> </ul> | <ul style="list-style-type: none"> <li>■ 1396 ms</li> <li>■ 1316 ms</li> </ul> |
| PMP75 | Max. | PMP71 + influence of the diaphragm seal                                                                          |                     |                                                                                |                                                                                |

*Read cycle (PLC)*

- Acyclic: typically 25/s
- Cyclic: typically 30/s (depending on the number and type of function blocks used in the closed-control loop)

*Cycle time (update time)*

Min. 200 ms

The cycle time in a bus segment in cyclic data communication depends on the number of devices, on the segment coupler used and on the internal PLC cycle time. A new measured value can be determined up to five times a second.

**Dynamic behavior, FOUNDATION Fieldbus**

A typical configuration for the macro cycle time (host system) of 1 s results in the following behavior:

| Type  |      | Measuring cell                                                                                                   | Dead time ( $t_1$ ) | Dead time ( $t_1$ ) + Time constant T63 ( $t_2$ )                        | Dead time ( $t_1$ ) + Time constant T90 ( $t_3$ )                        |
|-------|------|------------------------------------------------------------------------------------------------------------------|---------------------|--------------------------------------------------------------------------|--------------------------------------------------------------------------|
| PMP71 | Min. | <ul style="list-style-type: none"> <li>■ 400 mbar (6 psi)</li> <li>■ <math>\geq 1</math> bar (15 psi)</li> </ul> | 90                  | <ul style="list-style-type: none"> <li>■ 160</li> <li>■ 125</li> </ul>   | <ul style="list-style-type: none"> <li>■ 206</li> <li>■ 126</li> </ul>   |
|       | Max. | <ul style="list-style-type: none"> <li>■ 400 mbar (6 psi)</li> <li>■ <math>\geq 1</math> bar (15 psi)</li> </ul> | 1090                | <ul style="list-style-type: none"> <li>■ 1160</li> <li>■ 1125</li> </ul> | <ul style="list-style-type: none"> <li>■ 1206</li> <li>■ 1126</li> </ul> |
| PMP75 | Max. | PMP71 + influence of the diaphragm seal                                                                          |                     |                                                                          |                                                                          |

*Read cycle*

- Acyclic: typically 10/s
- Cyclic: max. 10/s (depending on the number and type of function blocks used in a closed-control loop)

*Cycle time (update time)*

Cyclic: min. 100 ms

## Installation factors

### Influence of installation position

PMP71: Device rotated 180°, process connection pointing upwards. The value is doubled for devices with inert oil.

- Process connection thread G 1 A, G 1 ½, G 2, 1 ½ MNPT, 2 MNPT, M 44x1.25, EN/DIN, ASME and JIS flanges: ≤ 10 mbar (0.15 psi).
- Process connection thread: G ½, ½ MNPT, JIS G ½, JIS R ½, M20x1.5: ≤ 4 mbar (0.06 psi).



A position-dependent zero point shift can be corrected. Please refer to the "Commissioning → Position adjustment" section of the Operating Instructions.

Different tightening torques (e.g. for Clamp or Varivent connections) can merely cause a shift in the zero point. This effect is corrected by position adjustment during commissioning.

### Warm-up period

- 4 to 20 mA HART: < 10 s
- PROFIBUS PA: 6 s
- FOUNDATION Fieldbus: 50 s

## Mounting

### General installation instructions

- For PMP75: →  115 "Installation instructions" section.
- A position-dependent zero point shift can be corrected directly at the device via operating keys, and also in hazardous areas in the case of devices with external operation. Depending on the installation location, diaphragm seals additionally shift the zero point by →  115.
- The device housing can be rotated up to 380°.
- Endress+Hauser offers a mounting bracket for installing the device on pipes or walls →  40.
- Use flushing rings for flange and cell diaphragm seals if buildup or clogging can be expected at the diaphragm seal connection. The flushing ring can be fitted between the process connection and diaphragm seal. Material buildup in front of the process membrane can be flushed away, and the pressure chamber vented, via the two lateral flushing holes.
- When measuring in media containing solids, such as dirty liquids, installing separators and drain valves is useful for capturing and removing sediment.
- Point the cable and plug downwards where possible to prevent moisture from entering (e.g. rain or condensation water).

### Measuring arrangement for devices without diaphragm seals – PMC71, PMP71

Cerabar S devices without diaphragm seals are mounted in accordance with the same guidelines as a manometer (DIN EN 837-2). We recommend the use of shutoff devices and siphons. The orientation depends on the measuring application.

#### Pressure measurement in gases

Mount the Cerabar S with shutoff device above the tapping point so that any condensate can flow into the process.

#### Pressure measurement in vapors

Use siphons for pressure measurement in steam. The siphon reduces the temperature to almost ambient temperature. Fill the siphon with liquid before commissioning. Preferably mount the Cerabar S with the siphon below the tapping point.

Advantages:

- defined water column only causes minimal/negligible measured errors
- only minimal/negligible thermal effects on the device

Mounting above the tapping point is also possible. Observe the max. permitted ambient temperature of the transmitter!

#### Pressure measurement in liquids

Mount the Cerabar S with shutoff device below or at the same level as the tapping point.

#### Level measurement

- Mount the Cerabar S below the lowest measuring point.
- Do not install the device in the following positions: In the filling curtain, in the tank outlet or at a point in the vessel which could be affected by pressure pulses from an agitator or a pump.
- The calibration and functional test can be carried out more easily if you mount the device downstream from a shutoff device.

### Measuring arrangement for devices with diaphragm seals – PMP75

→  115


### Orientation

The orientation may cause a zero point shift.

This position-dependent zero point shift can be corrected directly at the device via the operating key, and also in hazardous areas in the case of devices with external operation (position adjustment).

## Wall and pipe mounting, transmitter (optional)

Endress+Hauser offers the following mounting bracket for installing the device on pipes or walls:

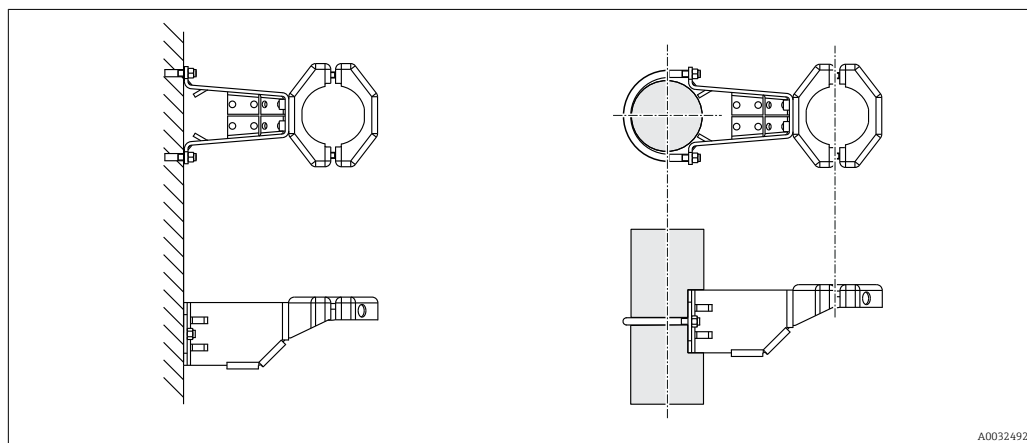


Ordering information:

- Product Configurator, order code for "Accessories enclosed", option "PA"
- For devices with separate housing (can be ordered using the order code for "Additional options 2") included in the scope of delivery
- Can be ordered as a separate accessory (part no.: 71102216).

For further details, see → 98.

## Wall and pipe mounting, valve manifold (optional)

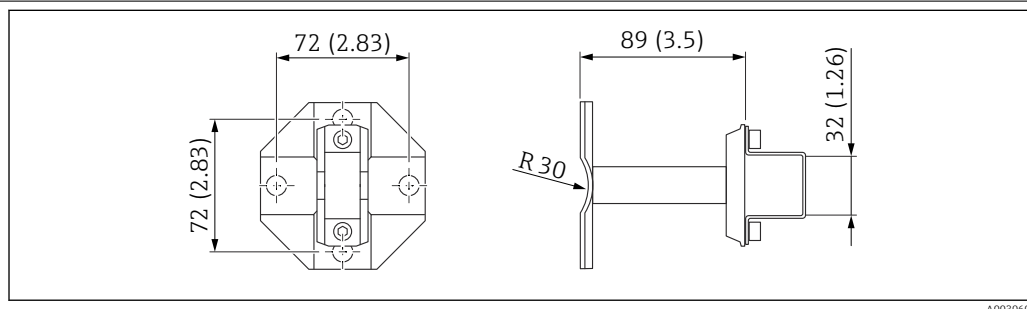

For the technical data (such as the dimensions or order numbers for screws), see the document SD01553P/00/EN.


Ordering information:

Product Configurator, order code for "Accessories enclosed", option "PK"

## Heat insulation – PMC71 high-temperature version

The PMC71 high-temperature version must only be insulated up to a certain height. The maximum permitted insulation height is indicated on the devices and applies to an insulation material with a heat conductivity  $\leq 0.04 \text{ W/(m x K)}$  and to the maximum permitted ambient and process temperature (see table below). The data were determined under the most critical application "quiescent air".

The data were determined under the most critical application "quiescent air".

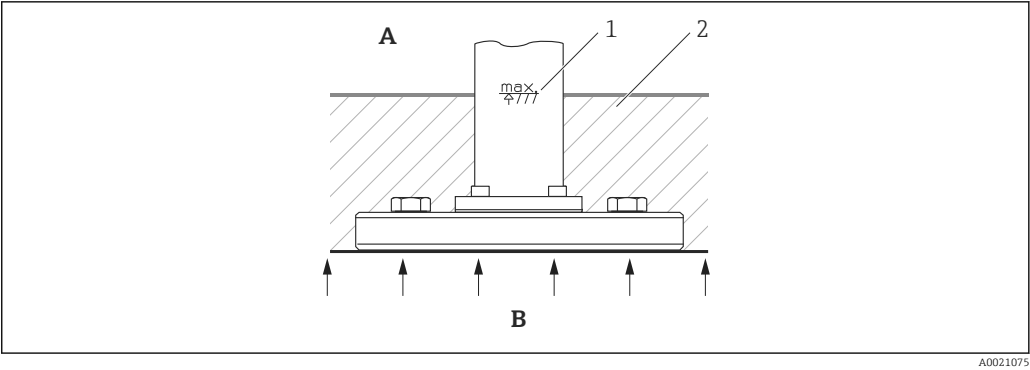

- A Ambient temperature range  
B Process temperature  
1 Insulation height  
2 Insulation material

|                           | Temperature       |
|---------------------------|-------------------|
| Ambient temperature range | ≤ 70 °C (158 °F)  |
| Process temperature       | ≤ 150 °C (302 °F) |

**Mounting of PVDF screw-in fittings**

**⚠ WARNING**

**Risk of damage to process connection!**

Risk of injury!

- ▶ PVDF threaded process connections must be mounted with the mounting bracket supplied!

The mounting bracket can be installed on pipes with a diameter of 1 ¼" to 2" or on walls.

Dimensions → 50.

**"Separate housing" version**

With the "separate housing" version, you are able to mount the housing with the electronics insert at a distance from the measuring point. This version facilitates trouble-free measurement

- Under particularly difficult measuring conditions (at installation locations that are cramped or difficult to access)
- If rapid cleaning of the measuring point is required and
- If the measuring point is exposed to vibrations.


You can choose between different cable versions:

- PE: 2 m (6.6 ft), 5 m (16 ft) and 10 m (33 ft)
- FEP: 5 m (16 ft).

Ordering information: Product Configurator, order code for "Additional options 2", version "G".

Dimensions →  98

In the case of the "separate housing" version, the sensor is delivered with the process connection and cable ready mounted. The housing and a mounting bracket are enclosed as separate units. The cable is provided with a socket at both ends. These sockets are simply connected to the housing and the sensor.

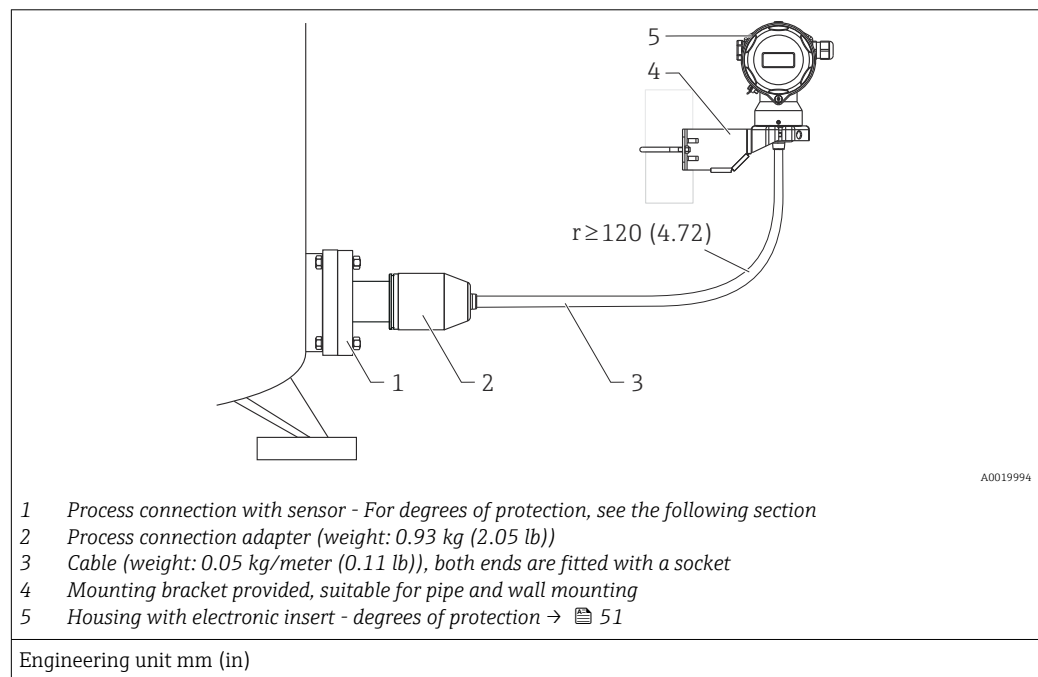

Degree of protection for the process connection and sensor with the use of

- FEP cable:
  - IP 69 <sup>1)</sup>
  - IP 66 NEMA 4/6P
  - IP 68 (1.83 mH<sub>2</sub>O for 24 h) NEMA 4/6P
- PE cable:
  - IP 66 NEMA 4/6P
  - IP 68 (1.83 mH<sub>2</sub>O for 24 h) NEMA 4/6P

Technical data of the PE and FEP cable:

- Minimum bending radius: 120 mm (4.72 in)
- Cable extraction force: max. 450 N (101.16 lbf)
- Resistance to UV light


Use in hazardous area:

- Intrinsically safe installations (Ex ia/IS)
- FM/CSA IS: for Div. 1 installation only

1) Designation of the IP protection class according to DIN EN 60529. Previous designation "IP69K" according to DIN 40050 Part 9 is no longer valid (standard withdrawn on November 1, 2012). The tests required by both standards are identical.

### Reduction of the installation height

If the separate housing is used, the installation height of the process connection is reduced compared to the dimensions of the standard version.

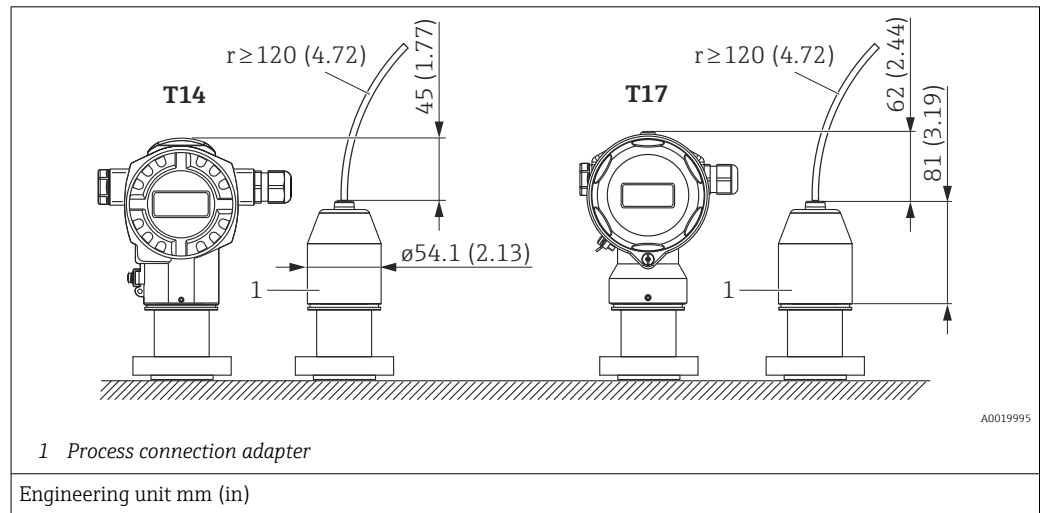


### Turning the housing

The housing can be rotated up to 360° by loosening the Allen screw.

#### Your benefits

- Easy installation due to optimum alignment of housing
- Good, accessible device operation
- Optimum readability of the onsite display (optional).

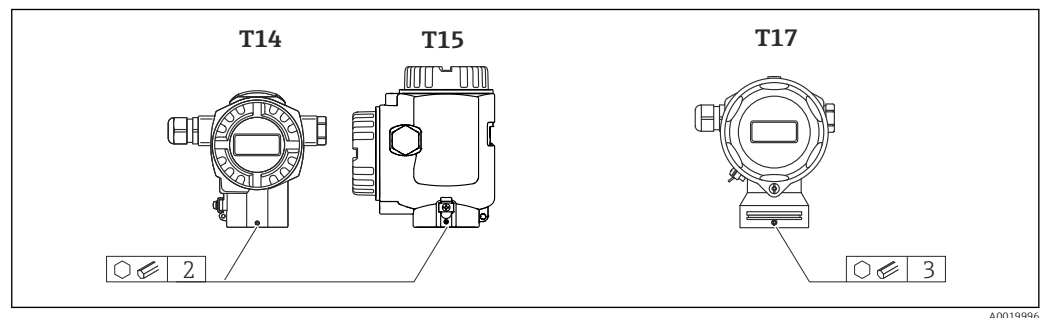

## Environment

### Ambient temperature range


| Version                                 | PMC71<br>High-temperature<br>version | PMC71                             | PMP71                                                                                        | PMP75   |
|-----------------------------------------|--------------------------------------|-----------------------------------|----------------------------------------------------------------------------------------------|---------|
| Without LCD display                     | -20 to +70 °C<br>(-4 to +158 °F)     | -40 to +85 °C<br>(-40 to +185 °F) | -50 to +85 °C (-58 to +185 °F) <sup>1)</sup><br>-60 to +85 °C (-76 to +185 °F) <sup>2)</sup> |         |
| With LCD display <sup>3)</sup>          |                                      | -20 to +70 °C (-4 to +158 °F)     |                                                                                              |         |
| With M12 plug,<br>elbowed               |                                      | -25 to +85 °C (-13 to +185 °F)    |                                                                                              |         |
| With separate<br>housing                | —                                    | -20 to +60 °C (-4 to +140 °F)     |                                                                                              | —       |
| Diaphragm seal<br>systems <sup>4)</sup> | —                                    | —                                 | —                                                                                            | → 📄 116 |
| MID parts certificate                   | —                                    | —                                 | -25 to +55 °C<br>(-13 to +131 °F)                                                            | —       |

- 1) If the temperature is below -40 °C (-40 °F), the chance of failure increases. Product Configurator, order code for "Test, Certificate" option "JN".
- 2) If the temperature is below -40 °C (-40 °F), the chance of failure increases. Product Configurator, order code for "Test, Certificate" option "JT".
- 3) Extended temperature application range (-50 to +85 °C (-58 to +185 °F)) with restrictions in optical properties, such as display speed and contrast
- 4) Ambient temperature range and process temperature range are mutually dependent - see "Heat insulation" section → ☞ 116

For high-temperature applications, either a PMP75 with a temperature isolator or with a capillary can be used. If vibrations also occur in the application, Endress+Hauser recommends using a PMP75 with a capillary. If a PMP75 with a temperature isolator or capillary is used, we recommend a suitable bracket for mounting (see "Wall and pipe mounting" section → ☞ 40).

### PMP71: Ambient temperature $T_a$ depending on the process temperature $T_p$

The process connection must be fully insulated for ambient temperatures below -40 °C (-40 °F).

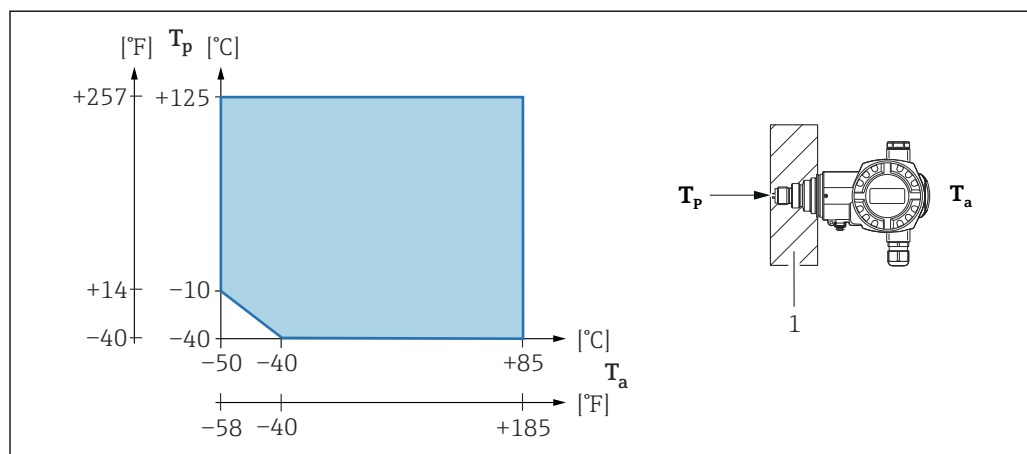

A0039403

1 Insulation material

**Hazardous area**

- For devices for use in hazardous areas, see Safety Instructions, Installation or Control Drawing.
- Pressure measuring instruments that have the usual explosion protection certificates (e.g. ATEX/CSA/FM/IEC Ex, etc) can be used in hazardous areas at ambient temperatures down to  $-50^{\circ}\text{C}$  ( $-58^{\circ}\text{F}$ ) (order code for "Test, Certificate" option "JN"). The functionality of the explosion protection is also guaranteed for ambient temperatures down to  $-50^{\circ}\text{C}$  ( $-58^{\circ}\text{F}$ ).
- Pressure measuring instruments that have the usual explosion protection certificates (e.g. ATEX-/IEC Ex, etc.) can be used in hazardous areas at ambient temperatures down to  $-60$  to  $+85^{\circ}\text{C}$  ( $-76$  to  $+185^{\circ}\text{F}$ ) (order code for "Test, Certificate" option "JT"). The functionality of the explosion protection is also guaranteed for ambient temperatures down to  $-50^{\circ}\text{C}$  ( $-58^{\circ}\text{F}$ ). At temperatures  $\leq -50^{\circ}\text{C}$  ( $-58^{\circ}\text{F}$ ), explosion protection is guaranteed by the housing in the case of flameproof enclosure (Ex d) type of protection. The functionality of the transmitter cannot be fully guaranteed.

**Storage temperature range**

- $-40$  to  $+90^{\circ}\text{C}$  ( $-40$  to  $+194^{\circ}\text{F}$ )  
Option  $-50$  to  $+90^{\circ}\text{C}$  ( $-58$  to  $+194^{\circ}\text{F}$ ) order code 580 "Test, Certificate" option "JN". If the temperature is below  $-40^{\circ}\text{C}$  ( $-40^{\circ}\text{F}$ ), the probability of a failure increases.
- Option  $-60$  to  $+90^{\circ}\text{C}$  ( $-76$  to  $+194^{\circ}\text{F}$ ) order code 580 "Test, Certificate" option "JT". If the temperature is below  $-40^{\circ}\text{C}$  ( $-40^{\circ}\text{F}$ ), the probability of a failure increases.
- Local display:  $-40$  to  $+85^{\circ}\text{C}$  ( $-40$  to  $+185^{\circ}\text{F}$ )
- Separate housing:  $-40$  to  $+60^{\circ}\text{C}$  ( $-40$  to  $+140^{\circ}\text{F}$ )
- Devices with PVC-armored capillary:  $-25$  to  $+80^{\circ}\text{C}$  ( $-13$  to  $+176^{\circ}\text{F}$ )

**Degree of protection**

- Depends on the deployed
- housing: →  51
  - separate housing: →  98

**Climate class**

Class 4K4H (air temperature:  $-20$  to  $+55^{\circ}\text{C}$  ( $-4$  to  $+131^{\circ}\text{F}$ ), relative humidity: 4 to 100 %) fulfilled as per DIN EN 60721-3-4 (condensation possible. With PMC71, avoid condensate in the device.)

**Electromagnetic compatibility**

- Electromagnetic compatibility as per EN 61326 and NAMUR recommendation EMC (NE21).
- With enhanced immunity against electromagnetic fields as per EN 61000-4-3: 30 V/m with closed cover (for devices with T14 housing)  
Increased interference immunity with 30 V/m not available for 1-5V DC. EMC interference immunity for 1-5V DC: 10 V/m
- Maximum deviation:  $< 0.5\%$  of span
- All EMC measurements were performed with a turn down (TD) = 2:1.
- Class E3 as per OIML R75-2

For further details refer to the Declaration of Conformity.

**Vibration resistance**

| Device/accessory                 | Test standard             | Vibration resistance                                                                                   |
|----------------------------------|---------------------------|--------------------------------------------------------------------------------------------------------|
| PMC71 <sup>1)</sup>              | GL                        | Guaranteed for<br>3 to 25 Hz: $\pm 1.6\text{ mm}$ (0.063 in);<br>25 to 100 Hz: 4 g<br>in all 3 axes    |
| PMP71                            |                           |                                                                                                        |
| PMP75 <sup>2) 3)</sup>           |                           |                                                                                                        |
| With mounting bracket            | IEC 62828-1 / IEC 61298-3 | Guaranteed for<br>10 to 60 Hz: $\pm 0.15\text{ mm}$ (0.0059 in);<br>60 to 500 Hz: 2 g<br>in all 3 axes |
| PMP71 with MID parts certificate | OIML R117-1               | Class M3                                                                                               |

1) Not for high-temperature version with Ex d[ia], CSA XP or FM XP

2) With aluminum T14 housing only

3) For applications with very high temperatures, a PMP75 with either a temperature isolator or a capillary can be used. If vibrations also occur in the application, Endress+Hauser recommends using a PMP75 with a capillary. If a PMP75 with a temperature isolator or capillary is used, it must be mounted with a mounting bracket

**Oxygen applications**

Oxygen and other gases can react explosively to oils, grease and plastics, such that, among other things, the following precautions must be taken:

- All components of the system, such as measuring instruments, must be cleaned in accordance with the BAM requirements.
- Depending on the materials used, a certain maximum temperature and a maximum pressure must not be exceeded for oxygen applications.

The devices that are suitable for gaseous oxygen applications are indicated by  $p_{\max}$  in the following table.

HB = Cleaned for oxygen service

| Order code for devices <sup>1)</sup> ,<br>Cleaned for oxygen applications                                                   | $p_{\max}$ for oxygen applications                                                                                                                                                                         | $T_{\max}$ for oxygen applications |
|-----------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------|
| PMC71 – * * * * * 2 * * or<br>PMC71 – * * * * * A * * HB,<br>Devices with measuring cells, nominal value < 10 bar (150 psi) | Over pressure limit (OPL) <sup>2) 3)</sup> of the measuring cell                                                                                                                                           | 60 °C (140 °F)                     |
| PMC71 – * * * * * 2 * *,<br>PMC71 – * * * * * A * * HB,<br>Devices with measuring cells, nominal value ≥ 10 bar (150 psi)   | 40 bar (600 psi)                                                                                                                                                                                           | 60 °C (140 °F)                     |
| PMP71 – * * * * * N * * or<br>PMP71 – * * * * * F * * HB                                                                    | Depends on the lowest-rated element, with regard to pressure, of the selected components: overpressure limit (OPL) of the sensor, process connection (1.5 x PN) or fill fluid (80 bar (1 200 psi))         | 60 °C (140 °F)                     |
| PMP75 – * * * * * N * * or<br>PMP75 – * * * * * F * * HB                                                                    | Depends on the lowest-rated element, with regard to pressure, of the selected components: overpressure limit (OPL) of the measuring cell, process connection (1.5 x PN) or fill fluid (80 bar (1 200 psi)) | 60 °C (140 °F)                     |

1) Devices only, not accessories or enclosed accessories.

2) Product Configurator, order code for "Sensor range; sensor over pressure limit (= OPL)"

3) PMC71 with PVDF thread: Only mount with the enclosed mounting bracket. MWP 10 bar (150 psi), OPL max. 15 bar (225 psi). Process temperature range –10 to +60 °C (+14 to +140 °F)

**PWIS-free applications**

Special cleaning of the transmitter to remove paint-wetting substances, for use in paint shops, for instance.

Ordering information:

Product Configurator, order code for "Seal", option "L" or "M".

**Ultrapure gas applications**

Endress+Hauser also offers device for special applications, such as for ultrapure gas, which have been cleaned of oil and grease. No special restrictions regarding the process conditions apply to these devices.

Ordering information:

- Product Configurator, order code for "Seal" or
- Product Configurator, order code for "Fill fluid".

**Hydrogen applications**

A **ceramic** process membrane or a **gold-plated** metallic process membrane offers universal protection against hydrogen diffusion, both in gas applications and in applications with aqueous solutions.

**Applications with hydrogen in aqueous solutions**

A **gold/rhodium-coated** metallic process membrane (AU/Rh) offers effective protection against hydrogen diffusion.

**Operation in very corrosive environment**

PMP75:

For corrosive environments (e.g. maritime environment / coastal areas), Endress+Hauser recommends the use of a PVC or PTFE armor for the capillaries (→ 103).

## Process

**Process temperature limits** For oxygen applications →  46

### PMC71 (with ceramic process membrane)

- -25 to +125 °C (-13 to +257 °F)
- High-temperature version: -25 to +150 °C (-13 to +302 °F); Product Configurator, order code for "Additional options 1", option "T".
- For saturated steam applications, use a device with a metallic process membrane, or provide a siphon for temperature isolation when installing.
- Observe the process temperature range of the seal in the following table.

| Seal                                                                                                                                                     | Notes                                                                            | Process temperature range                                         | Option <sup>1)</sup> |
|----------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------|-------------------------------------------------------------------|----------------------|
| FKM                                                                                                                                                      | —                                                                                | -25 to +125 °C (-13 to +257 °F)/<br>150 °C (302 °F) <sup>2)</sup> | A, L                 |
| EPDM 70                                                                                                                                                  | FDA 21CFR177.2600                                                                | -40 to +125 °C (-40 to +257 °F)/<br>150 °C (302 °F) <sup>2)</sup> | B                    |
| EPDM 331                                                                                                                                                 | FDA 21CFR177.2600;<br>3A Class II; USP Class VI<br>DVGW (UBA "KTW", W270), NSF61 | -20 to +125 °C (-4 to +257 °F)/<br>150 °C (302 °F) <sup>2)</sup>  | B <sup>3)</sup>      |
| FFKM Perlast G75LT                                                                                                                                       | —                                                                                | -20 to +125 °C (-4 to +257 °F)/<br>150 °C (302 °F) <sup>2)</sup>  | C                    |
| Kalrez, Compound 4079                                                                                                                                    | —                                                                                | +5 to +125 °C (+41 to +257 °F)/<br>150 °C (302 °F) <sup>2)</sup>  | D, M                 |
| Chemraz, Compound 505                                                                                                                                    | —                                                                                | -10 to +125 °C (+14 to +257 °F)/<br>150 °C (302 °F) <sup>2)</sup> | E                    |
| HNBR                                                                                                                                                     | FDA 21CFR177.2600;<br>3A Class II; KTW; AFNOR; BAM                               | -25 to +125 °C (-13 to +257 °F)                                   | F <sup>4)</sup>      |
| NBR                                                                                                                                                      | —                                                                                | -10 to +100 °C (+14 to +212 °F)                                   | F                    |
| FKM                                                                                                                                                      | FDA 21CFR177.2600                                                                | -5 to +125 °C (+23 to +257 °F)                                    | G                    |
| FKM                                                                                                                                                      | Cleaned of oil and grease                                                        | -10 to +125 °C (+14 to +257 °F)/<br>150 °C (302 °F) <sup>2)</sup> | 1                    |
| FKM                                                                                                                                                      | Cleaned for oxygen service                                                       | -10 to +60 °C (+14 to +140 °F)                                    | 2 or A <sup>5)</sup> |
| The process temperature ranges specified here refer to permanent application of the PMC71.<br>They may be exceeded for a short time (e.g. for cleaning). |                                                                                  |                                                                   |                      |

- 1) Product Configurator, order code for "Seal"
- 2) 150 °C (302 °F) for high-temperature version
- 3) In combination with order code for "Additional options 1" option "F" or with order code for "Process connection" option "MP", "MR", "TD", "TF", "TK" or "TR"
- 4) These seals are used for devices with 3A-approved process connections.
- 5) with option "HB", see Product Configurator, order code for "Service"

### Applications with changes in temperature

Extreme changes in temperature can result in temporary measurement errors. Temperature compensation occurs after a few minutes. Internal temperature compensation occurs more quickly the smaller the change in temperature and the longer the time interval involved.



For further information please contact your local Endress+Hauser Sales Center.

### PMP71 (with metallic process membrane)

| Designation                                                     | Limits                                                                 |
|-----------------------------------------------------------------|------------------------------------------------------------------------|
| Process connections with internal process membrane              | -40 to +125 °C (-40 to +257 °F)<br>(150 °C (302 °F) for max. one hour) |
| Process connections with flush process membrane <sup>1)</sup>   | -40 to +100 °C (-40 to +212 °F)                                        |
| Process connections with flush process membrane, G ½ A, M20x1.5 | -20 to +85 °C (-4 to +185 °F)                                          |

1) Process connection 1A, 1B, 1N, 1P: seal supplied up to -20 °C (-4 °F) process temperature

### PMP71 (with metallic process membrane) with MID parts certificate

-25 to +55 °C (-13 to +131 °F)

### PMP75 (with diaphragm seal)

- Depending on the design and depending on the diaphragm seal and fill fluid: -70 °C (-94 °F) up to +400 °C (+752 °F). Observe temperature application limits of diaphragm seal oil → 115.
- Please observe the maximum gauge pressure and maximum temperature.

#### Devices with PTFE-coated process membrane


The non-stick coating has excellent gliding properties and is used to protect the process membrane against abrasive media.

#### NOTICE

**The device can be damaged if the PTFE foil is used for anything other than the designated purpose!**

- ▶ The PTFE foil used is designed to protect the unit against abrasion. It does not provide protection against corrosive media.

For the range of application of the 0.25 mm (0.01 in) PTFE foil on an AISI 316L (1.4404/1.4435) process membrane, see the following graphic:

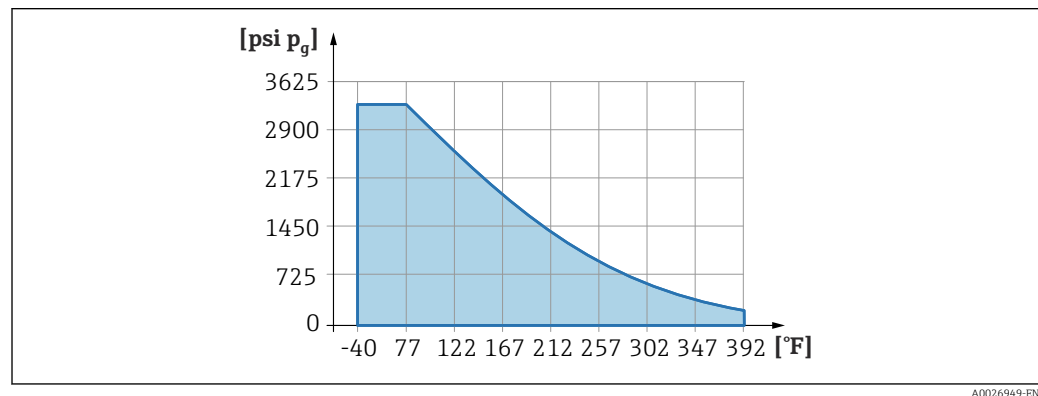

A0026949-EN


- For vacuum applications:  $p_{abs} \leq 1$  bar (14.5 psi) to 0.05 bar (0.725 psi) up to max. +150 °C (302 °F).

#### Diaphragm seal with tantalum process membrane

-70 to +300 °C (-94 to +572 °F)

#### Process temperature limits of capillary armoring: PMP75

- 316L: No restrictions
- PTFE: No restrictions
- PVC: See the following diagram

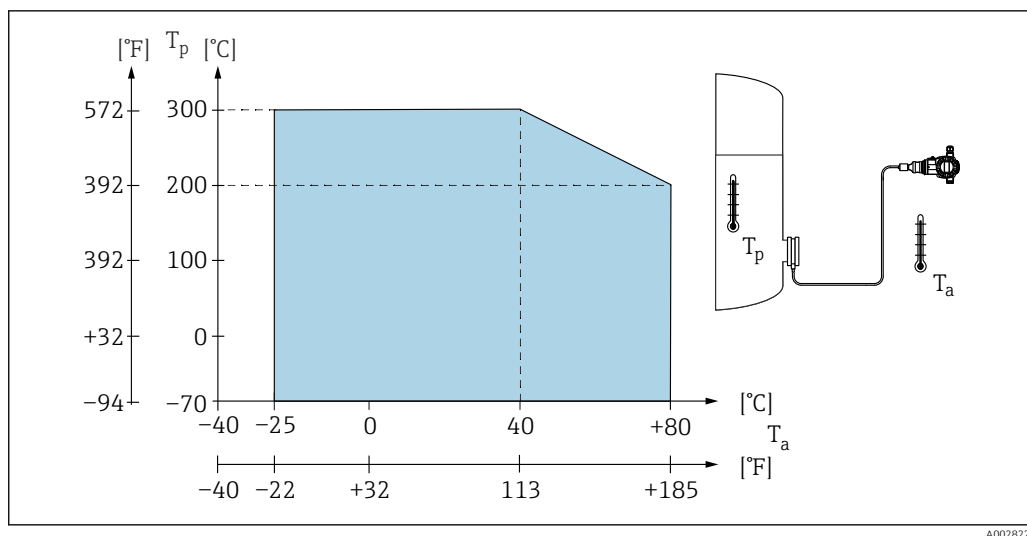

A0028220

## Pressure specifications

### ⚠ WARNING

**The maximum pressure for the measuring instrument depends on the lowest-rated element with regard to pressure.**

- ▶ For pressure specifications, see the "Measuring range" section and the "Mechanical construction" section.
- ▶ The measuring instrument must be operated only within the specified limits!
- ▶ MWP (maximum working pressure): The MWP (maximum working pressure) is specified on the nameplate. This value refers to a reference temperature of +20 °C (+68 °F) and may be applied to the device for an unlimited time. Observe the temperature dependency of the MWP. For the pressure values permitted at higher temperatures for flanges, please refer to standards EN 1092-1 (with regard to their stability-temperature property, the materials 1.4435 and 1.4404 are grouped together under EN 1092-1; the chemical composition of the two materials can be identical.), ASME B 16.5a, JIS B 2220 (the latest version of the standard applies in each case).
- ▶ The overload limit is the maximum pressure that a device may be subjected to during a test. It exceeds the maximum operating pressure by a certain factor. This value refers to a reference temperature of +20 °C (+68 °F).
- ▶ The Pressure Equipment Directive (2014/68/EU) uses the abbreviation "PS". The abbreviation "PS" corresponds to the MWP (maximum working pressure) of the measuring instrument.
- ▶ In the case of measuring cell range and process connection combinations where the overpressure limit (OPL) of the process connection is less than the nominal value of the measuring cell, the device is set at the factory, at the very maximum, to the OPL value of the process connection. If the entire measuring cell range must be used, select a process connection with a higher OPL value (1.5 x MWP; MWP = PN).
- ▶ In oxygen applications, the values for  $p_{\max}$  and  $T_{\max}$  for oxygen applications must not be exceeded → 46.
- ▶ Devices with ceramic process membrane: Avoid steam hammering! Steam hammering can cause zero point drift. Recommendation: Residue (such as condensation or drops of water) can remain on the process membrane after SIP cleaning and lead to local steam hammering if steam cleaning is performed again. In practice, drying the process membrane (e.g. by blowing off excess moisture) has proven to be a successful way of avoiding steam hammering.

## Burst pressure

| Device              | Measuring range                     | Burst pressure         |
|---------------------|-------------------------------------|------------------------|
| PMP71 <sup>1)</sup> | 400 mbar (6 psi)...10 bar (150 psi) | 100 bar (1 450 psi)    |
|                     | 40 bar (600 psi)                    | 250 bar (3 625 psi)    |
|                     | 100 bar (1 500 psi)                 | 1 000 bar (14 500 psi) |
|                     | 400 bar (6 000 psi)                 | 2 000 bar (29 000 psi) |
|                     | 700 bar (10 500 psi)                | 2 800 bar (40 600 psi) |

1) PMP75 with mounted diaphragm seal system, PMC71 with ceramic process membrane and the universal adapter process connection are exceptions.

## Mechanical construction

### Device height


The device height is calculated from

- the height of the housing
- the height of optional mounted parts such as temperature isolators or capillaries
- the height of the relevant process connection.

The individual heights of the components can be found in the following sections. To calculate the device height, simply add up the individual heights of the components. If necessary, the installation space (the space used to install the device) must also be taken into account. You can use the following table for this:

| Section                | Page     | Elevation | Example |
|------------------------|----------|-----------|---------|
| Height of housing      | → 51 ff. | (A)       |         |
| Optional mounted parts | → 75     | (B)       |         |
| Process connections    | → 54     | (H)       |         |
| Installation space     | -        | (I)       |         |
| Device height          |          |           |         |


A0021437

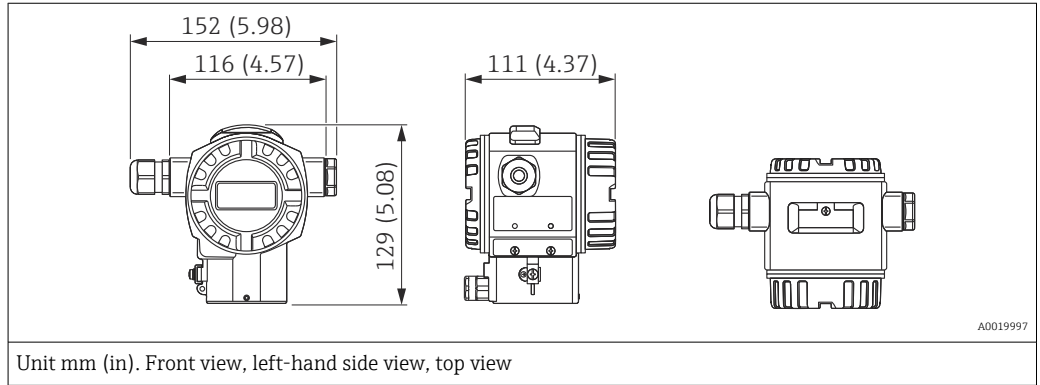**T14 housing, optional display on the side**


| Material               |            | Degree of protection | Cable entry        | Weight kg (lb) |                 | Option <sup>1)</sup> |
|------------------------|------------|----------------------|--------------------|----------------|-----------------|----------------------|
| Housing                | Cover seal |                      |                    | with display   | without display |                      |
| Aluminum <sup>2)</sup> | EPDM       | IP66/67 NEMA 6P      | M20 gland          | 1.2 (2.65)     | 1.1 (2.43)      | A                    |
|                        |            | IP66/67 NEMA 6P      | G ½" thread        |                |                 | B                    |
|                        |            | IP66/67 NEMA 6P      | NPT ½" thread      |                |                 | C                    |
|                        |            | IP66/67 NEMA 6P      | M12 plug           |                |                 | D                    |
|                        |            | IP66/67 NEMA 6P      | 7/8" plug          |                |                 | E                    |
|                        |            | IP65 NEMA 4          | HAN7D plug 90 deg. |                |                 | F                    |
|                        | FVMQ       | IP66/67 NEMA 6P      | M20 gland          |                |                 | G                    |
|                        | FVMQ       | IP66/67 NEMA 6P      | NPT ½" thread      |                |                 | H                    |
| 316L                   | EPDM       | IP66/67 NEMA 6P      | M20 gland          | 2.1 (4.63)     | 2.0 (4.41)      | 1                    |
|                        |            | IP66/67 NEMA 6P      | G ½" thread        |                |                 | 2                    |
|                        |            | IP66/67 NEMA 6P      | NPT ½" thread      |                |                 | 3                    |
|                        |            | IP66/67 NEMA 6P      | M12 plug           |                |                 | 4                    |
|                        |            | IP66/67 NEMA 6P      | 7/8" plug          |                |                 | 5                    |
|                        |            | IP65 NEMA 4          | HAN7D plug 90 deg. |                |                 | 6                    |
|                        | FVMQ       | IP66/67 NEMA 6P      | M20 gland          |                |                 | 7                    |
|                        | FVMQ       | IP66/67 NEMA 6P      | NPT ½" thread      |                |                 | 8                    |

1) Product Configurator, order code for "Housing, cover seal, cable entry, degree of protection"

2) Polyester powder coating on aluminum as per EN1706 AC43400 (reduced copper content ≤0.1 % to prevent corrosion)

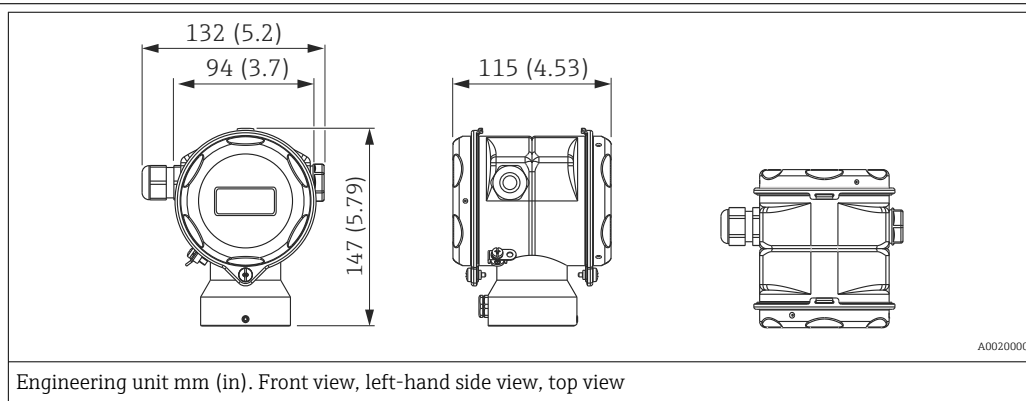**T17 housing (hygienic),  
optional display on the side**

| Material |            | Degree of protection <sup>1)</sup> | Cable entry   | Weight in kg (lb) |                 | Option <sup>2)</sup> |
|----------|------------|------------------------------------|---------------|-------------------|-----------------|----------------------|
| Housing  | Cover seal |                                    |               | with display      | without display |                      |
| 316L     | EPDM       | IP66/68 NEMA 6P                    | M20 gland     | 1.2 (2.65)        | 1.1 (2.43)      | R                    |
|          |            | IP66/68 NEMA 6P                    | G ½" thread   |                   |                 | S                    |
|          |            | IP66/68 NEMA 6P                    | NPT ½" thread |                   |                 | T                    |
|          |            | IP66/68 NEMA 6P                    | M12 plug      |                   |                 | U                    |
|          |            | IP66/68 NEMA 6P                    | 7/8" plug     |                   |                 | V                    |

1) Degree of protection IP 68: 1.83 mH<sub>2</sub>O for 24 h

2) Product Configurator, order code for "Housing, cover seal, cable entry, degree of protection"

**PMC71: height H**

| Process connection                                                         | Height H        |                  |
|----------------------------------------------------------------------------|-----------------|------------------|
|                                                                            | Standard        | Ex d version     |
| FNPT1/2<br>MNPT1/2<br>MNPT1/2 FNPT1/4<br>G1/2<br>M20x1.5<br>B0202<br>B0203 | 28 mm (1.1 in)  | 94 mm (3.7 in)   |
| MNPT1-1/2<br>MNPT2<br>G1-1/2<br>G2<br>M44x1.25                             | 59 mm (2.32 in) | 125 mm (4.92 in) |
| Flanges                                                                    | 83 mm (3.27 in) | 150 mm (5.91 in) |
| Hygienic process connections                                               | 90 mm (3.54 in) | 156 mm (6.14 in) |


| Process connection                                                                 | Height H                 |                                                 |
|------------------------------------------------------------------------------------|--------------------------|-------------------------------------------------|
|                                                                                    | High-temperature version | Ex d version including high-temperature version |
| FNPT1/2<br>MNPT1/2<br>MNPT1/2 FNPT1/4<br>G1/2<br>G1/2<br>M20x1.5<br>B0202<br>B0203 | 107 mm (4.21 in)         | 173 mm (6.81 in)                                |
| MNPT1-1/2<br>MNPT2<br>G1-1/2<br>G2<br>M44x1.25                                     | 59 mm (2.32 in)          | 125 mm (4.92 in)                                |
| Flanges                                                                            | 83 mm (3.27 in)          | 150 mm (5.91 in)                                |
| Hygienic process connections                                                       | 90 mm (3.54 in)          | 156 mm (6.14 in)                                |

**Explanation of terms**

- DN or NPS or A = alphanumeric designation of the flange size
- PN or Class or K = alphanumeric pressure rating of a component

# Process connections PMC71, internal process membrane

## ISO 228 G thread

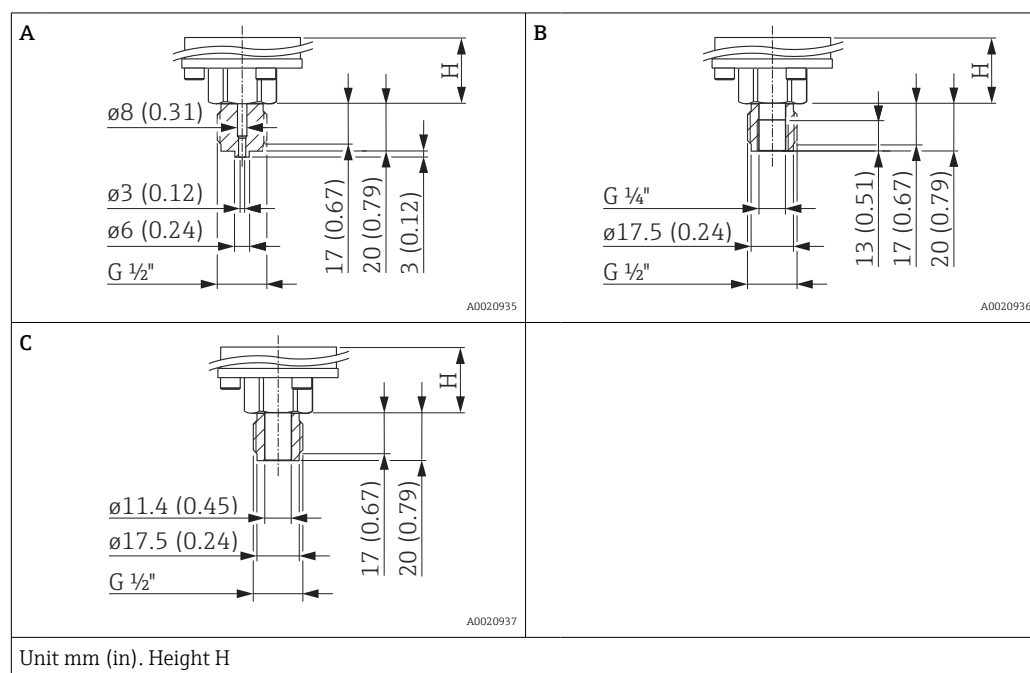


| Item | Designation                                        | Material                                                                                                                                                                                                                                   | Weight <sup>1)</sup> | Option <sup>2)</sup> |
|------|----------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------|----------------------|
|      |                                                    |                                                                                                                                                                                                                                            | kg (lb)              |                      |
| A    | ISO 228 G 1/2" A EN 837 thread                     | AISI 316L                                                                                                                                                                                                                                  | 0.60 (1.32)          | GA                   |
|      |                                                    | Alloy C276 (2.4819)                                                                                                                                                                                                                        |                      | GB                   |
|      |                                                    | Monel (2.4360)                                                                                                                                                                                                                             |                      | GC                   |
|      |                                                    | <b>PVDF</b><br><ul style="list-style-type: none"> <li>Only mount with a mounting bracket (included)</li> <li>MWP 10 bar (150 psi), OPL max. 15 bar (225 psi)</li> <li>Process temperature range: -10 to +60 °C (+14 to +140 °F)</li> </ul> |                      | GD                   |
| B    | ISO 228 G 1/2" A thread,<br>G 1/4" (female)        | AISI 316L                                                                                                                                                                                                                                  |                      | GE                   |
|      |                                                    | Alloy C276 (2.4819)                                                                                                                                                                                                                        |                      | GF                   |
|      |                                                    | Monel (2.4360)                                                                                                                                                                                                                             |                      | GG                   |
| C    | ISO 228 G 1/2" A thread,<br>Bore 11.4 mm (0.45 in) | AISI 316L                                                                                                                                                                                                                                  |                      | GH                   |
|      |                                                    | Alloy C276 (2.4819)                                                                                                                                                                                                                        |                      | GJ                   |
|      |                                                    | Monel (2.4360)                                                                                                                                                                                                                             |                      | GK                   |

1) Total weight consisting of measuring cell assembly and process connection.

2) Product Configurator, order code for "Process connection"

### ANSI thread

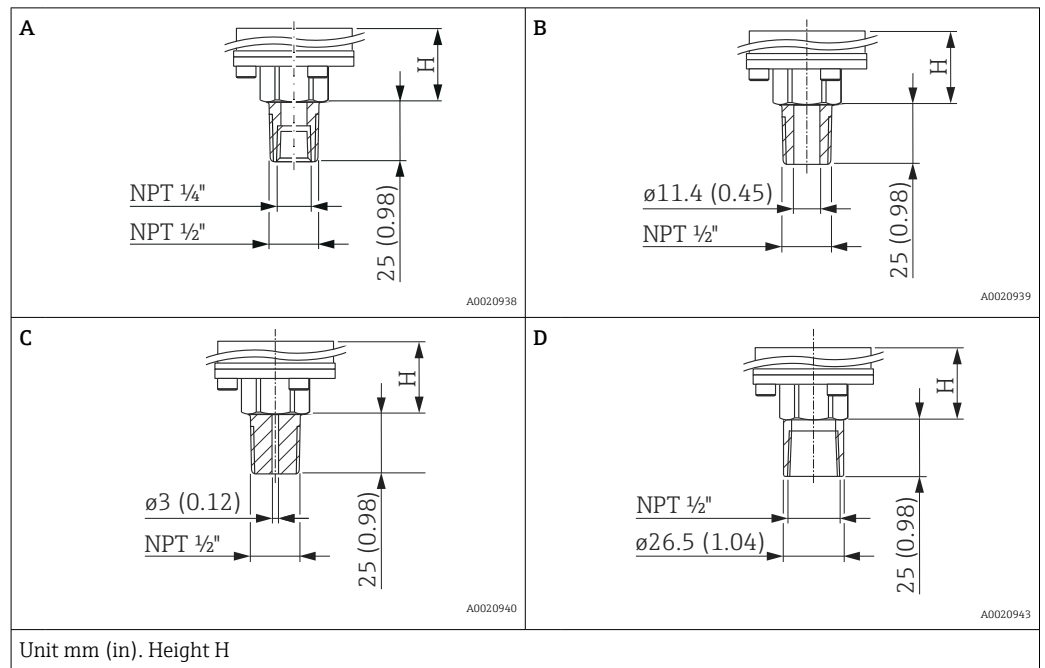


| Item | Designation                               | Material                                                                                                                                                                                                                                   | Weight <sup>1)</sup> | Option <sup>2)</sup> |
|------|-------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------|----------------------|
|      |                                           |                                                                                                                                                                                                                                            | kg (lb)              |                      |
| A    | ANSI 1/2" MNPT, 1/4" FNPT                 | AISI 316L                                                                                                                                                                                                                                  | 0.60 (1.32)          | RA                   |
|      |                                           | Alloy C276 (2.4819)                                                                                                                                                                                                                        |                      | RB                   |
|      |                                           | Monel (2.4360)                                                                                                                                                                                                                             |                      | RC                   |
| B    | ANSI 1/2" MNPT,<br>Bore 11.4 mm (0.45 in) | AISI 316L                                                                                                                                                                                                                                  |                      | RD                   |
|      |                                           | Alloy C276 (2.4819)                                                                                                                                                                                                                        |                      | RE                   |
|      |                                           | Monel (2.4360)                                                                                                                                                                                                                             |                      | RF                   |
| C    | ANSI 1/2" MNPT,<br>Bore 3 mm (0.12 in)    | <b>PVDF</b><br><ul style="list-style-type: none"> <li>Only mount with a mounting bracket (included)</li> <li>MWP 10 bar (150 psi), OPL max. 15 bar (225 psi)</li> <li>Process temperature range: +10 to +60 °C (+14 to +140 °F)</li> </ul> |                      | RG                   |
| D    | ANSI 1/2" FNPT<br>Bore 11.4 mm (0.45 in)  | AISI 316L                                                                                                                                                                                                                                  |                      | RH                   |
|      |                                           | Alloy C276 (2.4819)                                                                                                                                                                                                                        |                      | RJ                   |
|      |                                           | Monel (2.4360)                                                                                                                                                                                                                             |                      | RK                   |

1) Total weight consisting of measuring cell assembly and process connection.

2) Product Configurator, order code for "Process connection"

# Process connections PMC71, internal process membrane

## JIS thread

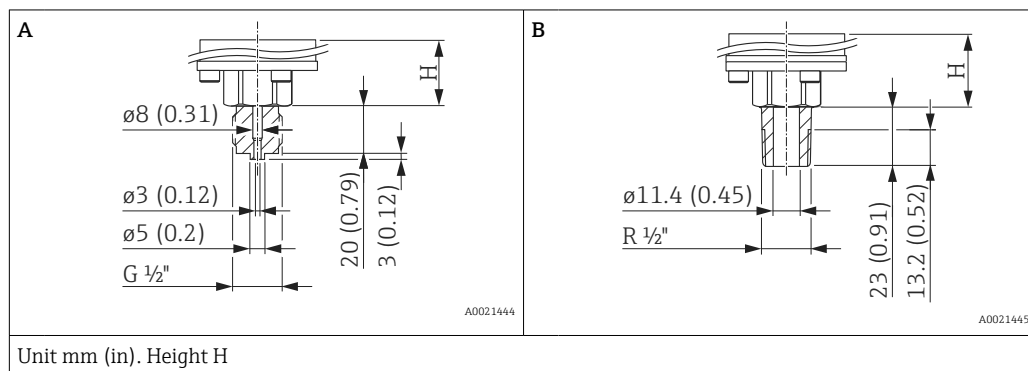


| Item | Designation             | Material  | Weight <sup>1)</sup> | Option <sup>2)</sup> |
|------|-------------------------|-----------|----------------------|----------------------|
|      |                         |           | kg (lb)              |                      |
| A    | JIS B0202 G 1/2" (male) | AISI 316L | 0.60 (1.32)          | GL                   |
| B    | JIS B0203 R 1/2" (male) |           |                      | RL                   |

1) Total weight consisting of measuring cell assembly and process connection.

2) Product Configurator, order code for "Process connection"

## DIN 13 thread

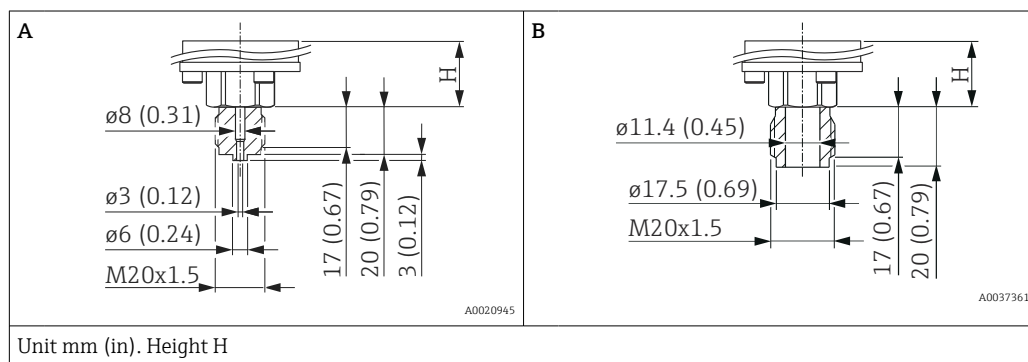


| Item | Designation                             | Material            | Weight <sup>1)</sup> | Option <sup>2)</sup> |
|------|-----------------------------------------|---------------------|----------------------|----------------------|
|      |                                         |                     | kg (lb)              |                      |
| A    | DIN 13 M20 x 1.5, EN 837 3 mm (0.12 in) | AISI 316L           | 0.60 (1.32)          | GP                   |
|      |                                         | Alloy C276 (2.4819) |                      | GQ                   |
| B    | DIN 13 M20 x 1.5 11.4 mm (0.45 in)      | AISI 316L           |                      | GR                   |

1) Total weight consisting of measuring cell assembly and process connection.

2) Product Configurator, order code for "Process connection"


Process connections PMC71, DIN 13 thread  
flush process membrane

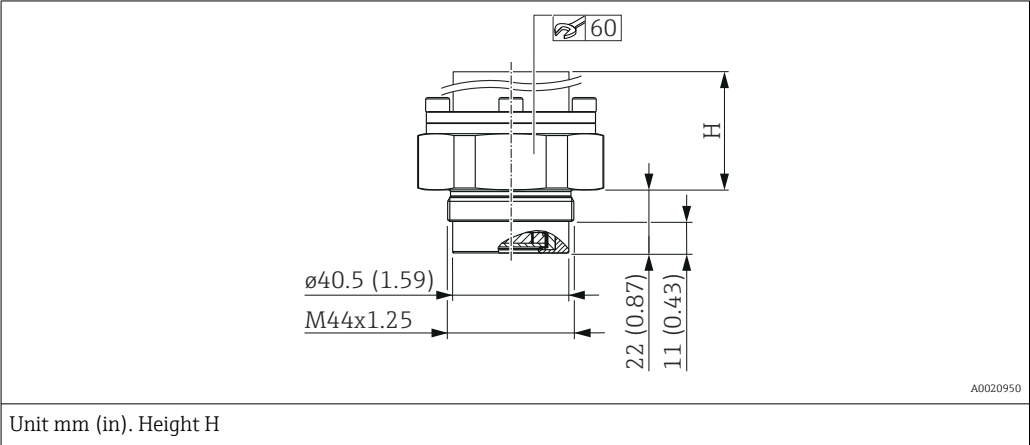

| Designation       | Material            | Weight      | Option <sup>1)</sup> |
|-------------------|---------------------|-------------|----------------------|
|                   |                     | kg (lb)     |                      |
| DIN 13 M44 x 1.25 | AISI 316L           | 0.63 (1.39) | 1R                   |
|                   | Alloy C276 (2.4819) |             | 1S                   |

1) Product Configurator, order code for "Process connection"

ISO 228 G thread

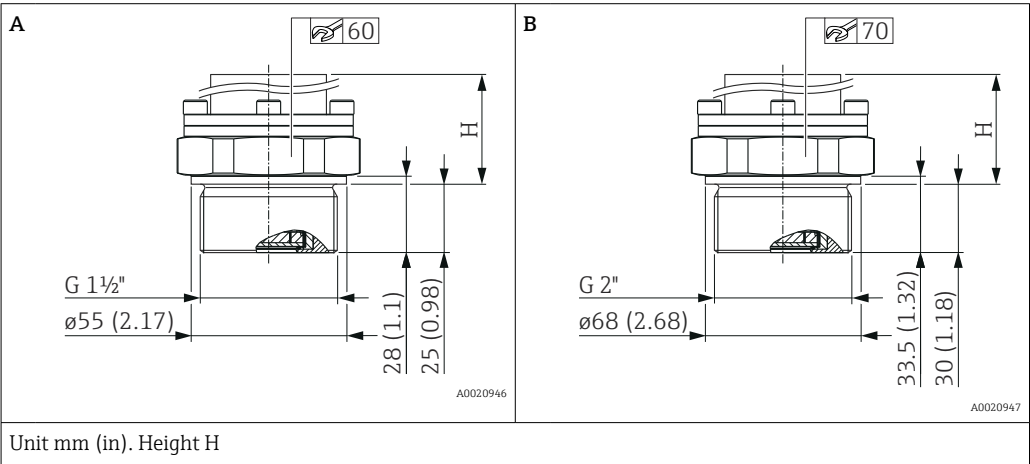


| Item | Designation               | Material            | Weight     | Option <sup>1)</sup> |
|------|---------------------------|---------------------|------------|----------------------|
|      |                           |                     | kg (lb)    |                      |
| A    | ISO 228 G 1 1/2" A thread | AISI 316L           | 0.8 (1.76) | 1G                   |
|      |                           | Alloy C276 (2.4819) | 0.9 (1.76) | 1H                   |
|      |                           | Monel (2.4360)      | 0.8 (1.76) | 1J                   |
| B    | ISO 228 G 2" A thread     | AISI 316L           | 1.2 (2.65) | 1K                   |
|      |                           | Alloy C276 (2.4819) | 1.2 (2.65) | 1L                   |
|      |                           | Monel (2.4360)      | 1.1 (2.43) | 1M                   |

1) Product Configurator, order code for "Process connection"

Process connections PMC71, flush process membrane

ANSI thread

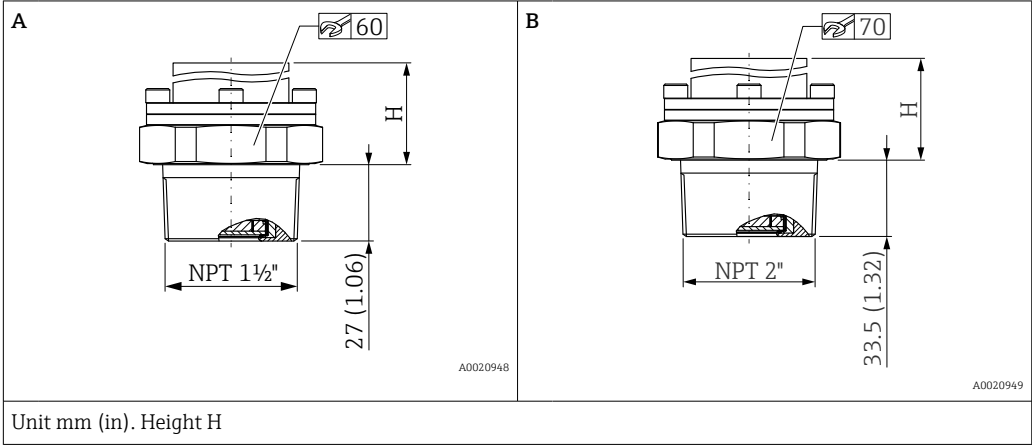


| Item | Designation      | Material            | Weight <sup>1)</sup> | Option <sup>2)</sup> |
|------|------------------|---------------------|----------------------|----------------------|
|      |                  |                     | kg (lb)              |                      |
| A    | ANSI 1 1/2" MNPT | AISI 316L           | 0.80 (1.76)          | 2D                   |
|      |                  | Alloy C276 (2.4819) |                      | 2E                   |
|      |                  | Monel (2.4360)      |                      | 2F                   |
| B    | ANSI 2" MNPT     | AISI 316L           | 1.20 (2.65)          | 2G                   |
|      |                  | Alloy C276 (2.4819) |                      | 2H                   |
|      |                  | Monel (2.4360)      |                      | 2J                   |

1) Total weight consisting of measuring cell assembly and process connection.

2) Product Configurator, order code for "Process connection"

# Process connections PMC71, flush process membrane

## EN flanges, connection dimensions as per EN 1092-1

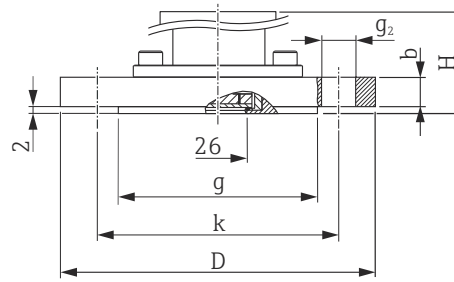

A0034684

*D* Diameter of flange  
*b* Thickness  
*g* Raised face  
*k* Pitch diameter  
*g<sub>2</sub>* Diameter of hole

Unit mm.


| Flange             |    |       |      |     |      |     | Boltholes |                |     | Weight <sup>1)</sup> | Option <sup>2)</sup> |
|--------------------|----|-------|------|-----|------|-----|-----------|----------------|-----|----------------------|----------------------|
| Material           | DN | PN    | Form | D   | b    | g   | Quantity  | g <sub>2</sub> | k   |                      |                      |
|                    |    |       |      | mm  | mm   | mm  |           | mm             | mm  | kg (lb)              |                      |
| AISI 316L          | 25 | 10-40 | B1   | 115 | 18   | 68  | 4         | 14             | 85  | 1.9 (4.19)           | BA                   |
| AISI 316L          | 32 | 10-40 | B1   | 140 | 18   | 78  | 4         | 18             | 100 | 2.5 (5.51)           | CP                   |
| AISI 316L          | 40 | 10-40 | B1   | 150 | 18   | 88  | 4         | 18             | 110 | 3.0 (6.62)           | CQ                   |
| AISI 316L          | 50 | 10-40 | B1   | 165 | 20   | 102 | 4         | 18             | 125 | 3.5 (7.72)           | B3                   |
| PVDF <sup>3)</sup> | 50 | 10-16 | B1   | 165 | 21.4 | 102 | 4         | 18             | 125 | 1.4 (3.09)           | BR                   |
| AISI 316L          | 50 | 63    | B2   | 180 | 26   | 102 | 4         | 22             | 135 | 4.6 (10.14)          | C3                   |
| PVDF <sup>3)</sup> | 80 | 10-16 | B1   | 200 | 21.4 | 138 | 8         | 18             | 160 | 1.9 (4.19)           | BS                   |
| AISI 316L          | 80 | 10-40 | B1   | 200 | 24   | 138 | 8         | 18             | 160 | 5.8 (12.79)          | B4                   |

1) Total weight consisting of measuring cell assembly and process connection.

2) Product Configurator, order code for "Process connection"

3) MWP 10 bar (150 psi), OPL max. 15 bar (225 psi); process temperature range: -10 to +60 °C (+14 to +140 °F)

## ASME flanges, connection dimensions as per ASME B 16.5, raised face RF

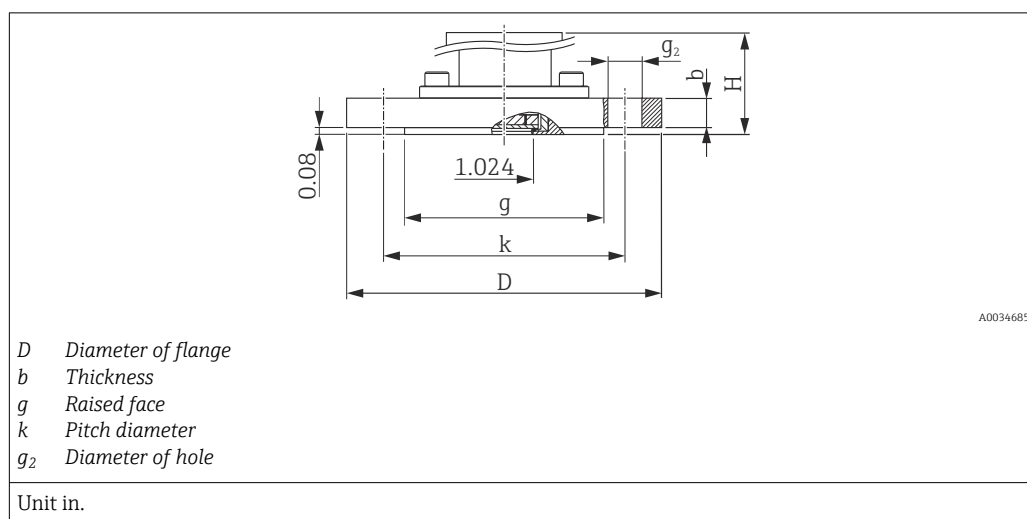

| Flange                      |      |             |      |      |      | Boltholes |                |      | Weight <sup>1)</sup> | Option <sup>2)</sup> |
|-----------------------------|------|-------------|------|------|------|-----------|----------------|------|----------------------|----------------------|
| Material                    | NPS  | Class       | D    | b    | g    | Quantity  | g <sub>2</sub> | k    |                      |                      |
|                             | [in] | [lb./sq.in] | [in] | [in] | [in] |           | [in]           | [in] | [kg (lb)]            |                      |
| AISI 316/316L <sup>3)</sup> | 1    | 150         | 4.25 | 1.18 | 2    | 4         | 0.62           | 3.12 | 2.3 (5.07)           | AA <sup>4)</sup>     |
| AISI 316/316L <sup>3)</sup> | 1    | 300         | 4.88 | 1.18 | 2    | 4         | 0.75           | 3.5  | 8.5 (18.74)          | AB <sup>4)</sup>     |
| AISI 316/316L <sup>3)</sup> | 1 ½  | 150         | 5    | 0.69 | 2.88 | 4         | 0.62           | 3.88 | 2.1 (4.63)           | AE                   |
| AISI 316/316L <sup>3)</sup> | 1 ½  | 300         | 6.12 | 0.81 | 2.88 | 4         | 0.88           | 4.5  | 3.3 (7.28)           | AQ                   |
| AISI 316/316L <sup>3)</sup> | 2    | 150         | 6    | 0.75 | 3.62 | 4         | 0.75           | 4.75 | 3.1 (6.84)           | AF                   |
| ECTFE <sup>5)</sup>         | 2    | 150         | 6    | 0.75 | 3.62 | 4         | 0.75           | 4.75 | 3.1 (6.84)           | JR                   |
| PVDF <sup>6)</sup>          | 2    | 150         | 6    | 0.75 | 3.62 | 4         | 0.75           | 4.75 | 0.5 (1.1)            | A3                   |
| AISI 316/316L <sup>3)</sup> | 2    | 300         | 6.5  | 0.88 | 3.62 | 8         | 0.75           | 5    | 4.0 (8.82)           | AR                   |
| AISI 316/316L <sup>3)</sup> | 3    | 150         | 7.5  | 0.94 | 5    | 4         | 0.75           | 6    | 5.7 (12.57)          | AG                   |
| ECTFE <sup>5)</sup>         | 3    | 150         | 7.5  | 0.94 | 5    | 4         | 0.75           | 6    | 5.7 (12.57)          | JS                   |
| PVDF <sup>6)</sup>          | 3    | 150         | 7.5  | 0.94 | 5    | 4         | 0.75           | 6    | 1.6 (3.53)           | A4                   |
| AISI 316/316L <sup>3)</sup> | 3    | 300         | 8.25 | 1.12 | 5    | 8         | 0.88           | 6.62 | 7.5 (16.54)          | AS                   |
| AISI 316/316L <sup>3)</sup> | 4    | 150         | 9    | 0.94 | 6.19 | 8         | 0.75           | 7.5  | 7.6 (16.76)          | AH                   |
| ECTFE <sup>5)</sup>         | 4    | 150         | 9    | 0.94 | 6.19 | 8         | 0.75           | 7.5  | 7.8 (17.20)          | JT                   |
| AISI 316/316L <sup>3)</sup> | 4    | 300         | 10   | 1.25 | 6.19 | 8         | 0.88           | 7.88 | 12.4 (27.34)         | AT                   |

1) Total weight consisting of measuring cell assembly and process connection.

2) Product Configurator, order code for "Process connection"


3) Combination of AISI 316 for required pressure resistance and AISI 316L for required chemical resistance (dual rated)

4) Screws must be 15 mm (0.59 in) longer than the standard flange screws

5) ECTFE coating on AISI 316/316L. When operating in hazardous areas, avoid electrostatic charging of the plastic surfaces.

6) MWP 10 bar (150 psi), OPL max. 15 bar (225 psi); process temperature range: -10 to +60 °C (+14 to +140 °F)

JIS flanges, connection dimensions in accordance with JIS B 2220 BL, raised face RF

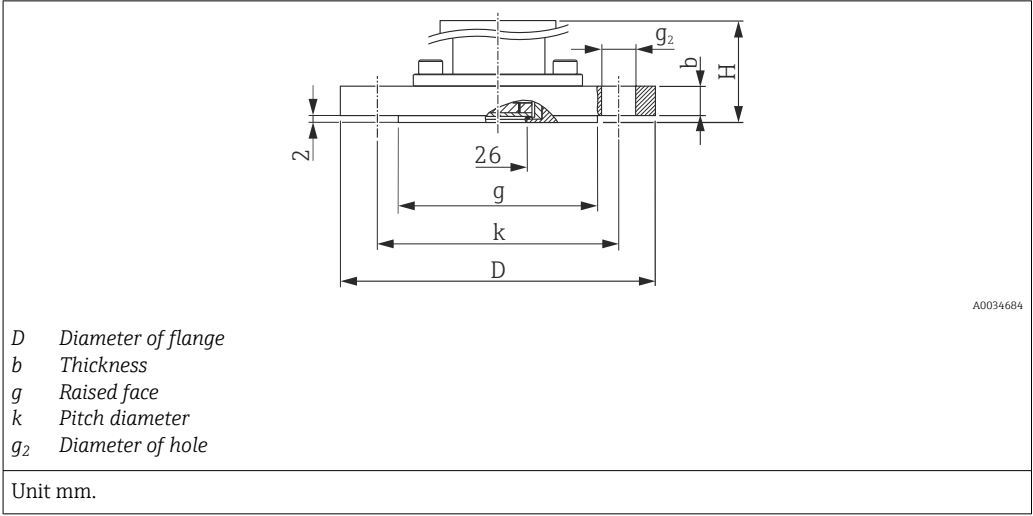


| Flange                |     |    |     |    |     | Boltholes |                |     | Weight <sup>1)</sup> | Option <sup>2)</sup> |
|-----------------------|-----|----|-----|----|-----|-----------|----------------|-----|----------------------|----------------------|
| Material              | A   | K  | D   | b  | g   | Quantity  | g <sub>2</sub> | k   |                      |                      |
|                       |     |    | mm  | mm | mm  |           | mm             | mm  | kg (lb)              |                      |
| AISI 316L<br>(1.4435) | 50  | 10 | 155 | 16 | 96  | 4         | 19             | 120 | 2.9 (6.39)           | KF                   |
|                       | 80  | 10 | 185 | 18 | 127 | 8         | 19             | 150 | 3.9 (8.60)           | KL                   |
|                       | 100 | 10 | 210 | 18 | 151 | 8         | 19             | 175 | 5.3 (11.69)          | KH                   |

1) Total weight consisting of measuring cell assembly and process connection.  
2) Product Configurator, order code for "Process connection"

Process connections PMC71,  
flush process membrane

China standard flanges, connection dimensions HG/T 20592-2009 (DN-flanges) or HG/T 20615-2009 ("-flanges), raised face RF

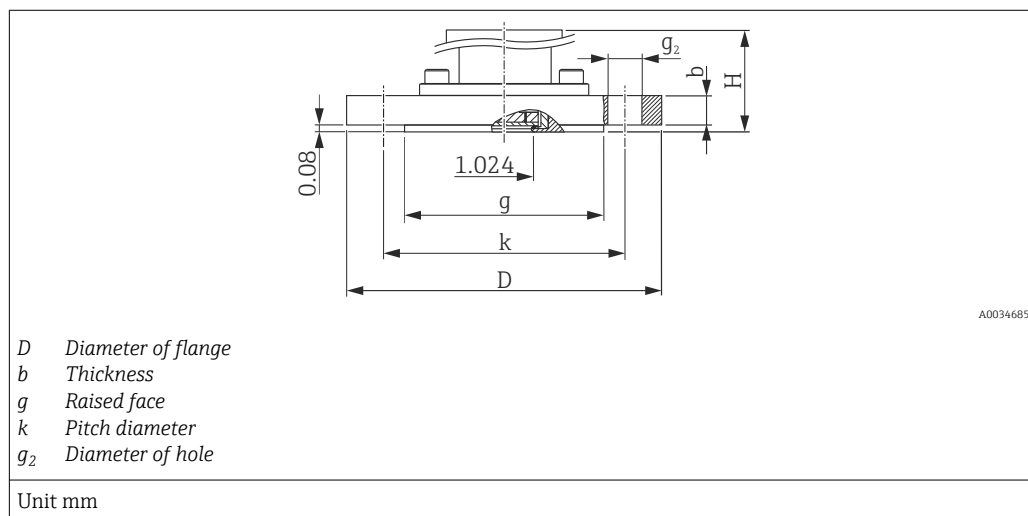

| Flange <sup>1)</sup> |        |      |      |      |      | Boltholes |                |      | Weight      | Option <sup>2)</sup> |
|----------------------|--------|------|------|------|------|-----------|----------------|------|-------------|----------------------|
| DN                   | PN     | D    | b    | g    | m    | Quantity  | g <sub>2</sub> | k    |             |                      |
|                      |        | [mm] | [mm] | [mm] | [mm] |           | [mm]           | [mm] | [kg (lb)]   |                      |
| 50                   | 40 bar | 165  | 20   | 102  | 27.5 | 4         | 18             | 125  | 3 (6.6)     | 7H                   |
| 80                   | 40 bar | 200  | 24   | 138  | 45.5 | 8         | 18             | 160  | 5.5 (12.13) | 7K                   |

1) Material: AISI 316L

2) Product Configurator, order code for "Process connection"

| Flange <sup>1)</sup> |               |      |      |      |       | Boltholes |                |       | Weight      | Option <sup>2)</sup> |
|----------------------|---------------|------|------|------|-------|-----------|----------------|-------|-------------|----------------------|
| NPS                  | Class         | D    | b    | g    | m     | Quantity  | g <sub>2</sub> | k     |             |                      |
|                      |               | [mm] | [mm] | [mm] | [mm]  |           | [mm]           | [mm]  | [kg (lb)]   |                      |
| 2"                   | 150lb./sq.in  | 150  | 17.5 | 92.1 | 22.55 | 4         | 18             | 120.7 | 2.2 (4.85)  | 7P                   |
| 2"                   | 300 lb./sq.in | 165  | 20.7 | 92.1 | 22.55 | 8         | 18             | 127   | 3 (6.62)    | 7R                   |
| 3"                   | 150 lb./sq.in | 190  | 22.3 | 127  | 40    | 4         | 18             | 152.4 | 4.7 (10.36) | 7V                   |
| 3"                   | 300 lb./sq.in | 210  | 27   | 127  | 40    | 8         | 22             | 168.3 | 6.6 (14.55) | 7X                   |


1) Material: AISI 316L

2) Product Configurator, order code for "Process connection"

PMC71 hygiene


Hygienic process connections, flush process membrane

Many process connections with an EPDM or HNBR seal are approved for the PMC71 in accordance with the guidelines of the 3A Sanitary Standard. To ensure the 3A approval for the PMC71 version is valid, a 3A-approved process connection must be selected in combination with an EPDM or HNBR seal when ordering (Product Configurator, order code for "Seal", option B or F).

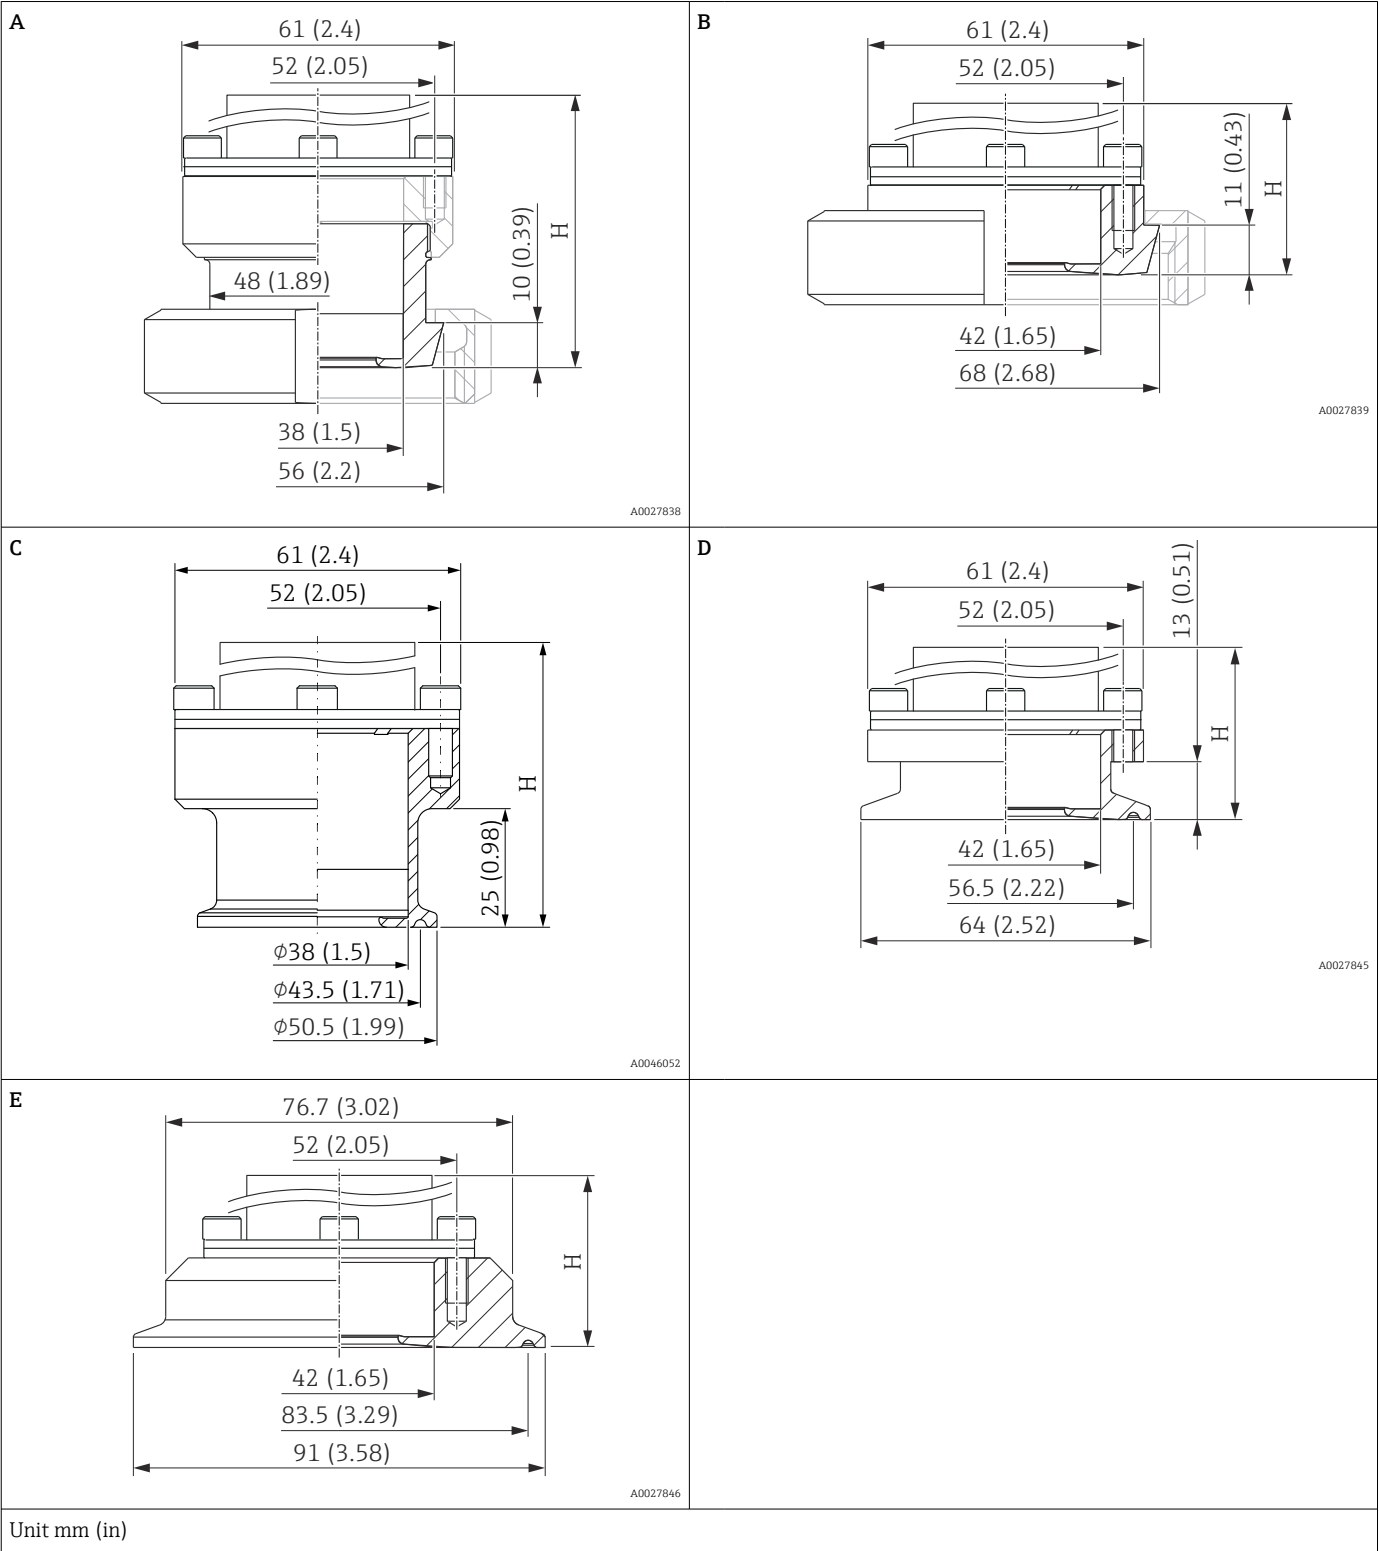

| Item | Designation                                | DN          | PN               | Material <sup>1)</sup> | Weight                | Option <sup>2)</sup> |
|------|--------------------------------------------|-------------|------------------|------------------------|-----------------------|----------------------|
|      |                                            |             |                  |                        | kg (lb) <sup>3)</sup> |                      |
| A    | DIN 11851, with HNBR or EPDM seal          | 40          | 25               | AISI 316L<br>(1.4435)  | 1.3 (2.87)            | MP <sup>4)</sup>     |
| B    | DIN 11851, with HNBR or EPDM seal          | 50          | 25               |                        | 1.27 (2.80)           | MR <sup>4)</sup>     |
| C    | Tri-Clamp ISO 2852, DIN32676               | 38 (1 1/2") | 40 <sup>5)</sup> |                        | 0.95 (2.09)           | TJ                   |
| D    | Tri-Clamp ISO 2852, with HNBR or EPDM seal | 51 (2")     | 40 <sup>5)</sup> |                        | 0.83 (1.83)           | TD                   |
| E    | Tri-Clamp ISO 2852, with NBR or EPDM seal  | 76.1 (3")   | 40 <sup>5)</sup> |                        | 1.2 (2.65)            | TF                   |

- 1) Delta ferrite content < 1 %. Roughness of wetted surfaces  $R_a < 0.76 \mu\text{m}$  (29.9  $\mu\text{in}$ ) as standard. Lower surface roughness available on request.
- 2) Product Configurator, order code for "Process connection"
- 3) Total weight consisting of the measuring cell assembly and the process connection.
- 4) Endress+Hauser supplies these slotted nuts in stainless steel AISI 304 (DIN/EN material number 1.4301) or in AISI 304L (DIN/EN material number 1.4307).
- 5) Restricted nominal pressure (13.8 bar (200 psi)) for the following approvals: Product Configurator, order code for "Approval", option "E", "U" and "V".

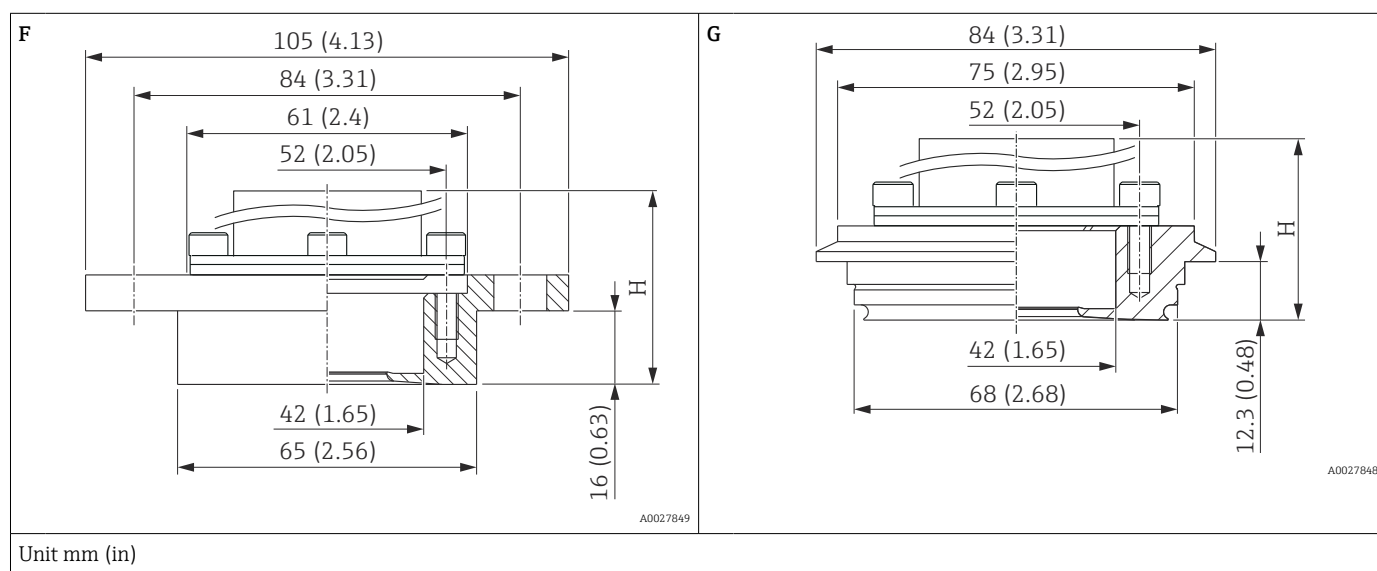


| Item | Designation                                                   | DN         | PN | Material <sup>1)</sup> | Weight                | Option <sup>2)</sup> |
|------|---------------------------------------------------------------|------------|----|------------------------|-----------------------|----------------------|
|      |                                                               |            |    |                        | kg (lb) <sup>3)</sup> |                      |
| F    | DRD<br>Slip-on flange<br>with HNBR or EPDM seal               | 50 (65 mm) | 25 | AISI 316L<br>(1.4435)  | 1.28 (2.82)           | TK                   |
| G    | Varivent type N for pipes 40 – 162,<br>with HNBR or EPDM seal | -          | 40 |                        | 1.09 (2.40)           | TR <sup>4)</sup>     |

- 1) Delta ferrite content < 1 %. Roughness of wetted surfaces  $R_a < 0.76 \mu\text{m}$  (29.9  $\mu\text{in}$ ) as standard. Lower surface roughness available on request.
- 2) Product Configurator, order code for "Process connection"
- 3) Total weight consisting of the measuring cell assembly and the process connection.
- 4) Endress+Hauser supplies these slotted nuts in stainless steel AISI 304 (DIN/EN material number 1.4301) or in AISI 304L (DIN/EN material number 1.4307).



# Process connections PMP71, internal process membrane

## ANSI thread

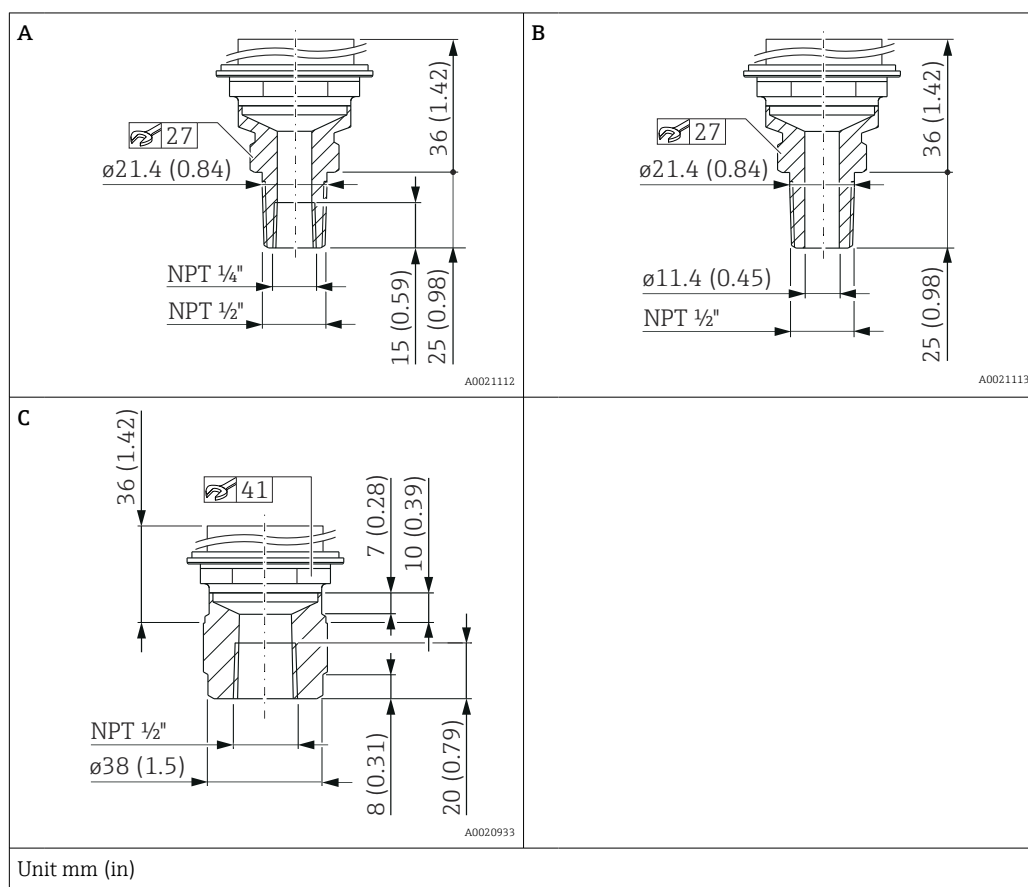


| Item | Designation                                                                                                     | Material            | Weight      | Option <sup>1)</sup> |
|------|-----------------------------------------------------------------------------------------------------------------|---------------------|-------------|----------------------|
|      |                                                                                                                 |                     | kg (lb)     |                      |
| A    | ANSI 1/2" MNPT, 1/4" FNPT                                                                                       | AISI 316L           | 0.63 (1.39) | RA                   |
|      |                                                                                                                 | Alloy C276 (2.4819) |             | RB                   |
| B    | ANSI 1/2" MNPT,<br>Bore 11.4 mm (0.45 in) = 400 bar (6 000 psi)<br>Bore 3.2 mm (0.13 in) = 700 bar (10 500 psi) | AISI 316L           |             | RD                   |
|      |                                                                                                                 | Alloy C276 (2.4819) |             | RE                   |
| C    | ANSI 1/2" FNPT                                                                                                  | AISI 316L           | 0.7 (1.54)  | RH                   |
|      |                                                                                                                 | Alloy C276 (2.4819) |             | RJ                   |

1) Product Configurator, order code for "Process connection"

Process connections PMP71,  
internal process membrane


JIS thread

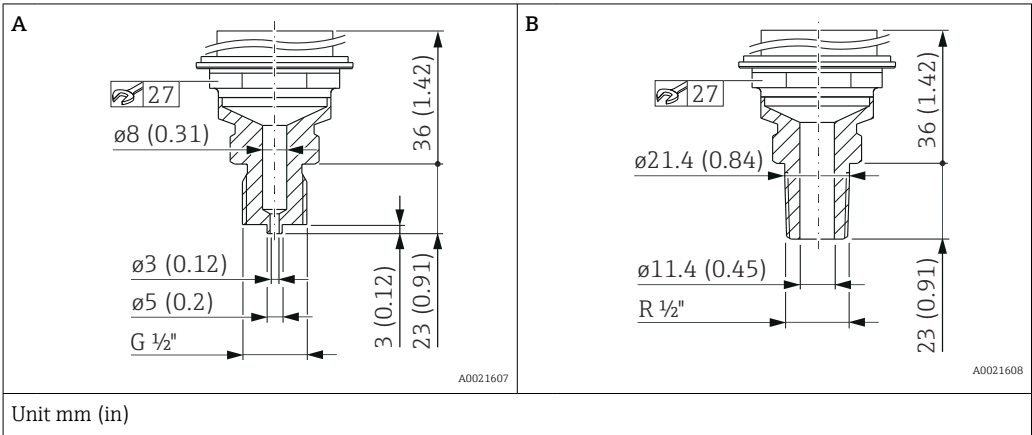

| Item | Designation             | Material  | Weight     | Option <sup>1)</sup> |
|------|-------------------------|-----------|------------|----------------------|
|      |                         |           | kg (lb)    |                      |
| A    | JIS B0202 G 1/2" (male) | AISI 316L | 0.6 (1.32) | GL                   |
| B    | JIS B0203 R 1/2" (male) |           |            | RL                   |

1) Product Configurator, order code for "Process connection"

DIN 13 thread

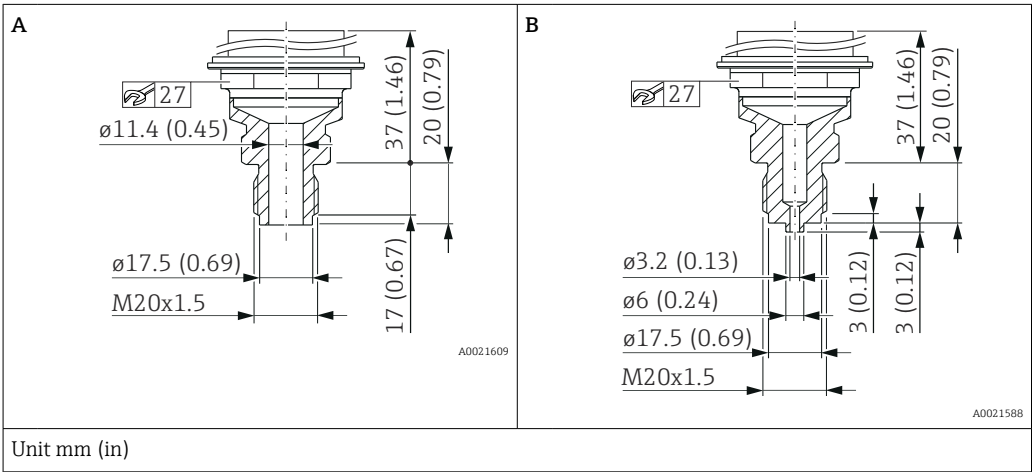


| Item | Designation                             | Material            | Weight     | Option <sup>1)</sup> |
|------|-----------------------------------------|---------------------|------------|----------------------|
|      |                                         |                     | kg (lb)    |                      |
| A    | DIN 13 M20 x 1.5 11.4 mm (0.45 in)      | AISI 316L           | 0.6 (1.32) | GP                   |
|      |                                         | Alloy C276 (2.4819) |            | GQ                   |
| B    | DIN 13 M20 x 1.5, EN 837 3 mm (0.12 in) | AISI 316L           |            | GR                   |
|      |                                         | Alloy C276 (2.4819) |            | GS                   |

1) Product Configurator, order code for "Process connection"

# Process connections PMP71, flush process membrane


## ISO 228 G thread

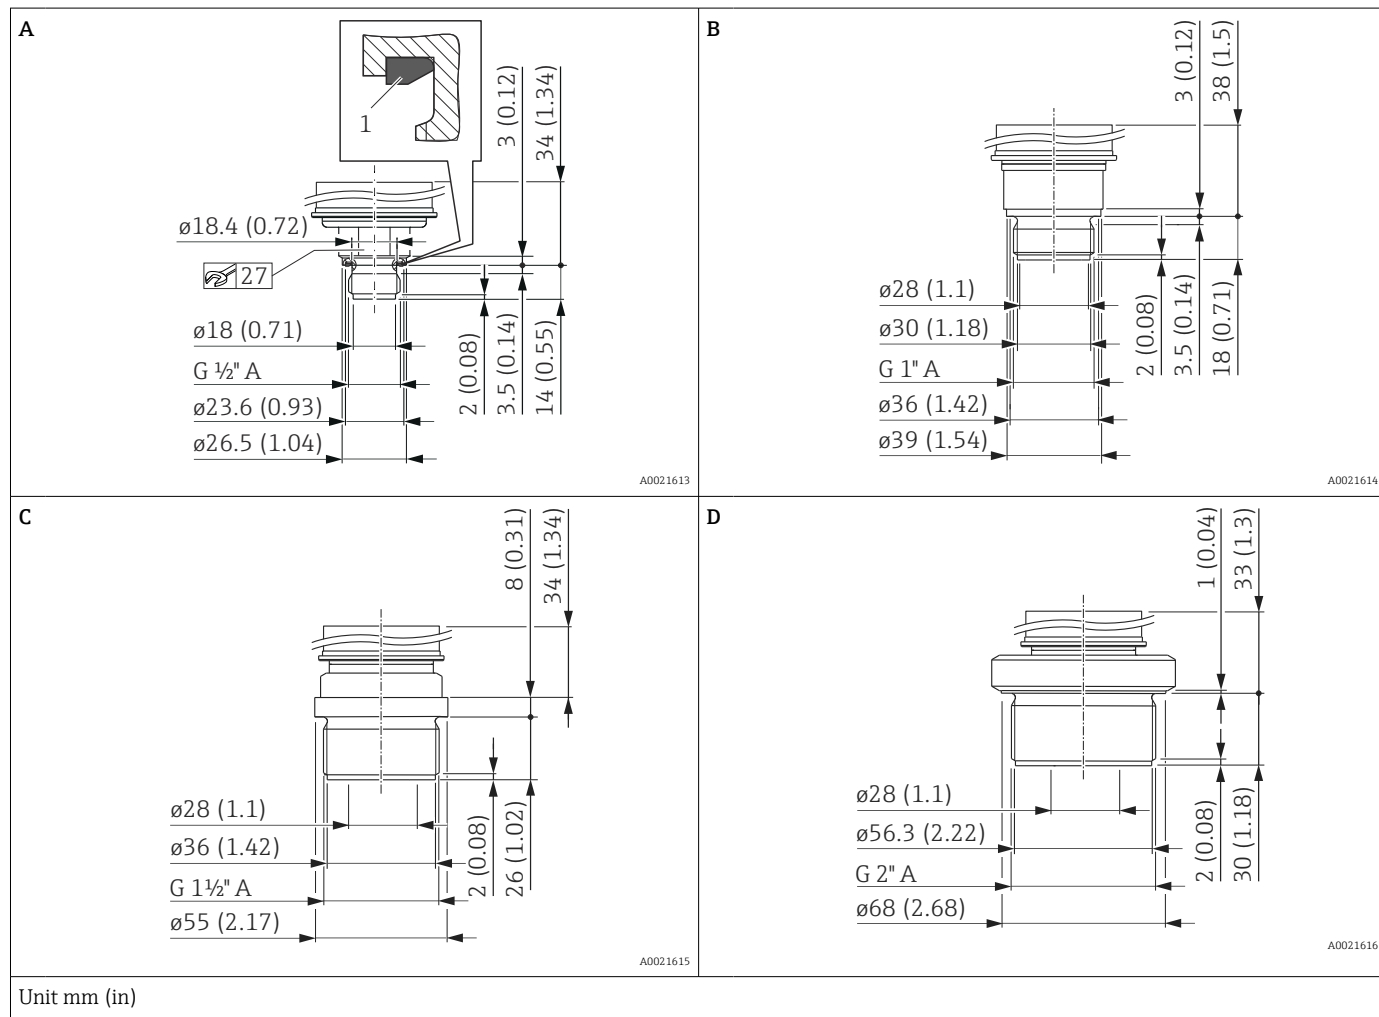

| Item | Designation                                                               | Material            | Weight     | Option <sup>1)</sup> |
|------|---------------------------------------------------------------------------|---------------------|------------|----------------------|
|      |                                                                           |                     | kg (lb)    |                      |
| A    | ISO 228 G 1/2" A thread, DIN 3852<br>FKM form seal (item 1) pre-installed | AISI 316L           | 0.4 (0.88) | 1A                   |
|      |                                                                           | Alloy C276 (2.4819) |            | 1B                   |
| B    | ISO 228 G 1" A thread                                                     | AISI 316L           | 0.7 (1.54) | 1D                   |
|      |                                                                           | Alloy C276 (2.4819) |            | 1E                   |
| C    | ISO 228 G 1 1/2" A thread                                                 | AISI 316L           | 1.1 (2.43) | 1G                   |
|      |                                                                           | Alloy C276 (2.4819) |            | 1H                   |
| D    | ISO 228 G 2" A thread                                                     | AISI 316L           | 1.5 (3.31) | 1K                   |
|      |                                                                           | Alloy C276 (2.4819) |            | 1L                   |


1) Product Configurator, order code for "Process connection"

DIN thread

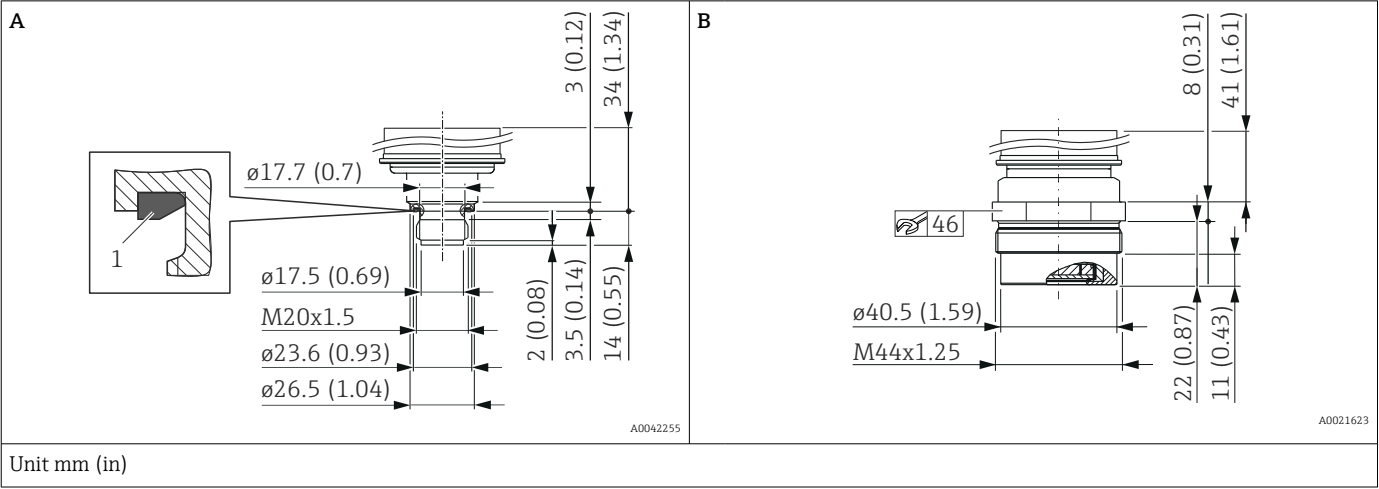

| Item | Designation                                                           | Material            | Weight     | Option <sup>1)</sup> |
|------|-----------------------------------------------------------------------|---------------------|------------|----------------------|
|      |                                                                       |                     | kg (lb)    |                      |
| A    | DIN 16288 M20 x 1.5 thread<br>FKM 80 flat seal (item 1) pre-installed | AISI 316L           | 0.4 (0.88) | 1N                   |
|      |                                                                       | Alloy C276 (2.4819) |            | 1P                   |
| B    | DIN 13 M44 x 1.25 thread                                              | AISI 316L           | 1.1 (2.43) | 1R                   |
|      |                                                                       | Alloy C276 (2.4819) |            | 1S                   |

1) Product Configurator, order code for "Process connection"

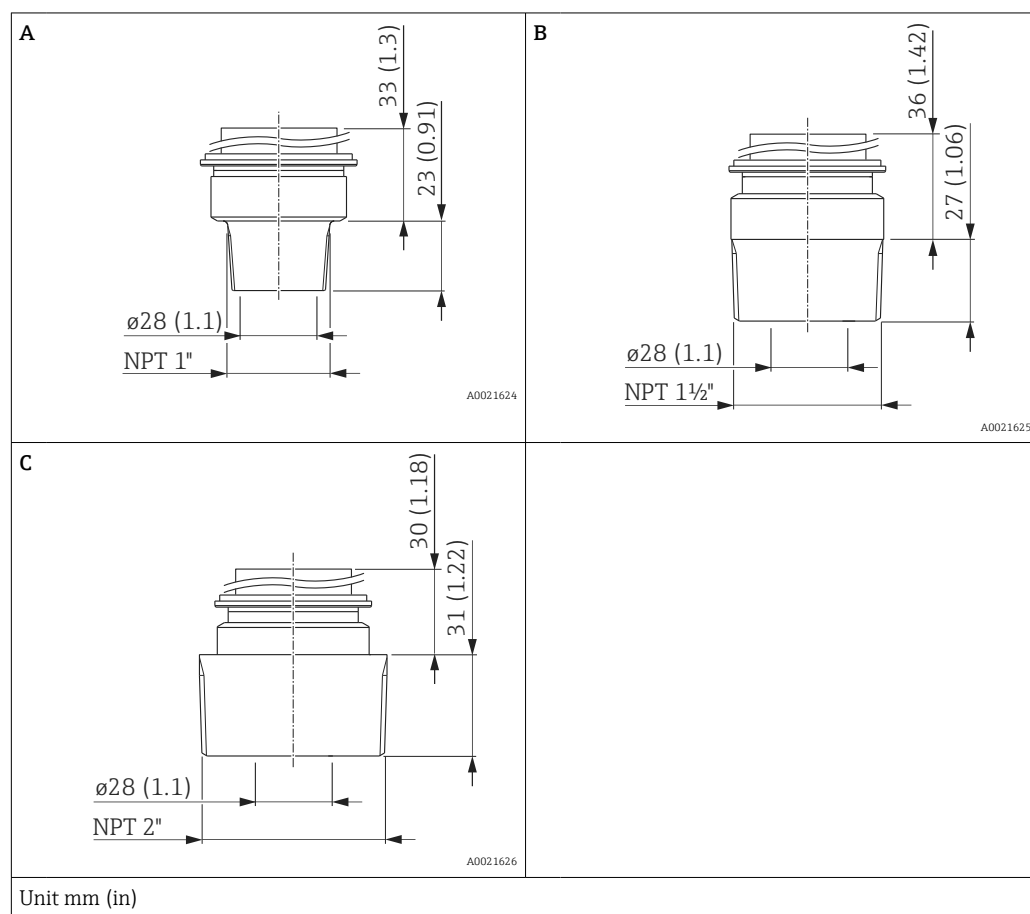
**Process connections PMP71,  
flush process membrane**
**ANSI thread**


| Item | Designation    | Material            | Weight     | Option <sup>1)</sup> |
|------|----------------|---------------------|------------|----------------------|
|      |                |                     | kg (lb)    |                      |
| A    | ANSI 1" MNPT   | AISI 316L           | 0.7 (1.54) | 2A                   |
|      |                | Alloy C276 (2.4819) |            | 2B                   |
| B    | ANSI 1 ½" MNPT | AISI 316L           | 1 (2.21)   | 2D                   |
|      |                | Alloy C276 (2.4819) |            | 2E                   |
| C    | ANSI 2" MNPT   | AISI 316L           | 1.3 (2.87) | 2G                   |
|      |                | Alloy C276 (2.4819) |            | 2H                   |

1) Product Configurator, order code for "Process connection"

# Process connections PMP71, flush process membrane

## EN flanges, connection dimensions as per EN 1092-1

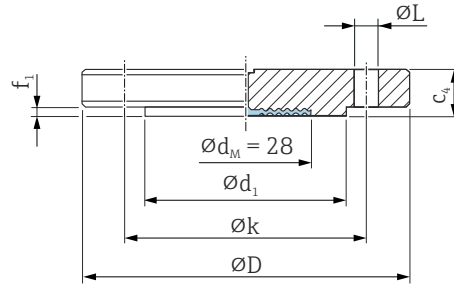

A0045473


$\varnothing D$  Diameter of flange  
 $c_4$  Thickness  
 $\varnothing d_1$  Raised face  
 $f_1$  Raised face  
 $\varnothing k$  Pitch diameter  
 $\varnothing L$  Diameter of hole  
 $\varnothing d_M$  Max. diameter of process membrane

Unit mm

| Flange <sup>1)</sup> |       |      |                 |       |                   |       | Boltholes |                 |                 | Weight<br>Flange | Option <sup>2)</sup> |
|----------------------|-------|------|-----------------|-------|-------------------|-------|-----------|-----------------|-----------------|------------------|----------------------|
| DN                   | PN    | Form | $\varnothing D$ | $c_4$ | $\varnothing d_1$ | $f_1$ | Quantity  | $\varnothing L$ | $\varnothing k$ |                  |                      |
|                      |       |      | mm              | mm    | mm                | mm    |           | mm              | mm              | kg (lb)          |                      |
| 25                   | 10-40 | B1   | 115             | 18    | 68                | 2     | 4         | 14              | 85              | 1.38<br>(3.04)   | CN                   |
| 32                   | 10-40 | B1   | 140             | 18    | 78                | 2     | 4         | 18              | 100             | 2.03<br>(4.48)   | CP                   |
| 40                   | 10-40 | B1   | 150             | 18    | 88                | 3     | 4         | 18              | 110             | 2.35<br>(5.18)   | CQ                   |
| 50                   | 10-40 | B1   | 165             | 20    | 102               | 3     | 4         | 18              | 125             | 3.2 (7.06)       | B3                   |
| 80                   | 10-40 | B1   | 200             | 24    | 138               | 3     | 8         | 18              | 160             | 5.54<br>(12.22)  | B4                   |

1) Material: AISI 316L

2) Product Configurator, order code for "Process connection"

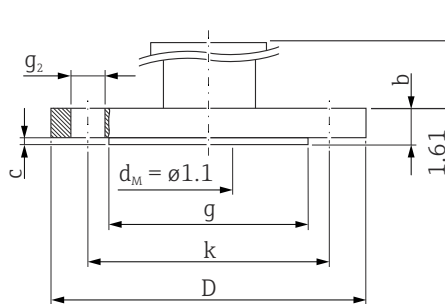**Process connections PMP71,  
flush process membrane**
**ASME flanges, connection dimensions as per ASME B 16.5, raised face RF**


A0022645

*D* Diameter of flange  
*b* Thickness  
*g* Raised face  
*c* Thickness of raised face  
*k* Pitch diameter  
*g<sub>2</sub>* Diameter of hole  
*d<sub>M</sub>* Max. diameter of process membrane


Unit in.

| Flange <sup>1)</sup> |           |      |      |      |      | Boltholes |                |      | Weight       | Option <sup>2)</sup> |
|----------------------|-----------|------|------|------|------|-----------|----------------|------|--------------|----------------------|
| NPS                  | Class     | D    | b    | g    | c    | Quantity  | g <sub>2</sub> | k    |              |                      |
| [in]                 | lb./sq.in | [in] | [in] | [in] | [in] |           | [in]           | [in] |              |                      |
| 1                    | 150       | 4.25 | 0.61 | 2.44 | 0.08 | 4         | 0.62           | 3.13 | 1.1 (2.43)   | AA                   |
| 1                    | 300       | 4.88 | 0.69 | 2.70 | 0.06 | 4         | 0.75           | 3.5  | 1.3 (2.87)   | AN                   |
| 1 ½                  | 150       | 5    | 0.69 | 2.88 | 0.08 | 4         | 0.62           | 3.88 | 1.5 (3.31)   | AE                   |
| 1 ½                  | 300       | 6.12 | 0.81 | 2.88 | 0.08 | 4         | 0.88           | 4.5  | 2.6 (5.73)   | AQ                   |
| 2                    | 150       | 6    | 0.75 | 3.62 | 0.08 | 4         | 0.75           | 4.75 | 2.4 (5.29)   | AF                   |
| 2                    | 300       | 6.5  | 0.88 | 3.62 | 0.08 | 8         | 0.75           | 5    | 3.2 (7.06)   | AR                   |
| 3                    | 150       | 7.5  | 0.94 | 5    | 0.08 | 4         | 0.75           | 6    | 4.9 (10.8)   | AG                   |
| 3                    | 300       | 8.25 | 1.12 | 5    | 0.08 | 8         | 0.88           | 6.62 | 6.7 (14.77)  | AS                   |
| 4                    | 150       | 9    | 0.94 | 6.19 | 0.08 | 8         | 0.75           | 7.5  | 7.1 (15.66)  | AH                   |
| 4                    | 300       | 10   | 1.25 | 6.19 | 0.08 | 8         | 0.88           | 7.88 | 11.6 (25.88) | AT                   |

1) Material: AISI 316/316L; Combination of AISI 316 for required pressure resistance and AISI 316L for required chemical resistance (dual rated)

2) Product Configurator, order code for "Process connection"

Process connections PMP71, flush process membrane JIS flanges, connection dimensions in accordance with JIS B 2220 BL, raised face RF

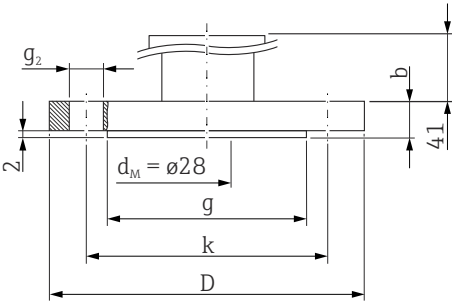

A0022643

*D* Diameter of flange  
*b* Thickness  
*g* Raised face  
*k* Pitch diameter  
*g<sub>2</sub>* Diameter of hole  
*ød<sub>M</sub>* Max. diameter of process membrane


Unit mm

| Flange    |     |    |      |      |      | Boltholes |                |      | Weight<br>Flange | Option <sup>1)</sup> |
|-----------|-----|----|------|------|------|-----------|----------------|------|------------------|----------------------|
| Material  | A   | K  | D    | b    | g    | Quantity  | g <sub>2</sub> | k    |                  |                      |
|           |     |    | [mm] | [mm] | [mm] |           | [mm]           | [mm] | [kg]             |                      |
| AISI 316L | 25  | 20 | 125  | 16   | 67   | 4         | 19             | 90   | 1.5 (3.31)       | KA                   |
| AISI 316L | 50  | 10 | 155  | 16   | 96   | 4         | 19             | 120  | 2.0 (4.41)       | KF                   |
| AISI 316L | 80  | 10 | 185  | 18   | 127  | 8         | 19             | 150  | 3.3 (7.28)       | KL                   |
| AISI 316L | 100 | 10 | 210  | 18   | 151  | 8         | 19             | 175  | 4.4 (9.7)        | KH                   |

1) Product Configurator, order code for "Process connection"

Process connections PMP71,  
flush process membrane

China standard flanges, connection dimensions HG/T 20592-2009 (DN-flanges) or HG/T 20615-2009 ("-flanges), raised face RF

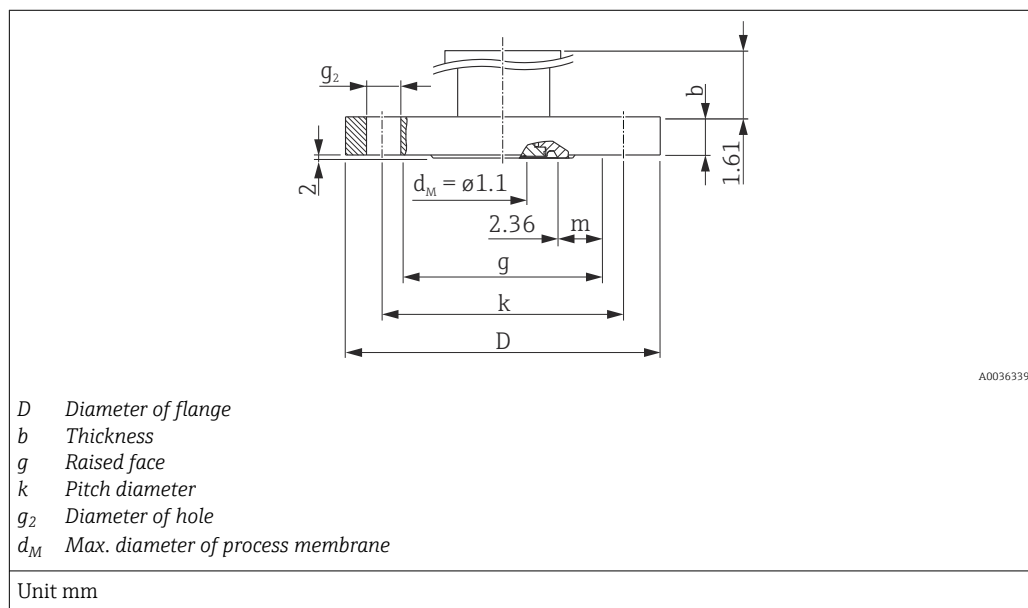

| Flange <sup>1)</sup> |        |      |      |      |      | Boltholes |       |      | Weight      | Option <sup>2)</sup> |
|----------------------|--------|------|------|------|------|-----------|-------|------|-------------|----------------------|
| DN                   | PN     | D    | b    | g    | m    | Quantity  | $g_2$ | k    |             |                      |
|                      |        | [mm] | [mm] | [mm] | [mm] |           | [mm]  | [mm] | [kg (lb)]   |                      |
| 50                   | 40 bar | 165  | 20   | 102  | 27.5 | 4         | 18    | 125  | 3 (6.6)     | 7H                   |
| 80                   | 40 bar | 200  | 24   | 138  | 45.5 | 8         | 18    | 160  | 5.5 (12.13) | 7K                   |

1) Material: AISI 316L


2) Product Configurator, order code for "Process connection"

| Flange <sup>1)</sup> |               |      |      |      |       | Boltholes |       |       | Weight      | Option <sup>2)</sup> |
|----------------------|---------------|------|------|------|-------|-----------|-------|-------|-------------|----------------------|
| NPS                  | Class         | D    | b    | g    | m     | Quantity  | $g_2$ | k     |             |                      |
|                      |               | [mm] | [mm] | [mm] | [mm]  |           | [mm]  | [mm]  | [kg (lb)]   |                      |
| 2"                   | 150lb./sq.in  | 150  | 17.5 | 92.1 | 22.55 | 4         | 18    | 120.7 | 2.2 (4.85)  | 7P                   |
| 2"                   | 300 lb./sq.in | 165  | 20.7 | 92.1 | 22.55 | 8         | 18    | 127   | 3 (6.62)    | 7R                   |
| 3"                   | 150 lb./sq.in | 190  | 22.3 | 127  | 40    | 4         | 18    | 152.4 | 4.7 (10.36) | 7V                   |
| 3"                   | 300 lb./sq.in | 210  | 27   | 127  | 40    | 8         | 22    | 168.3 | 6.6 (14.55) | 7X                   |

1) Material: AISI 316L

2) Product Configurator, order code for "Process connection"


Process connections PMP71      **Oval flange**

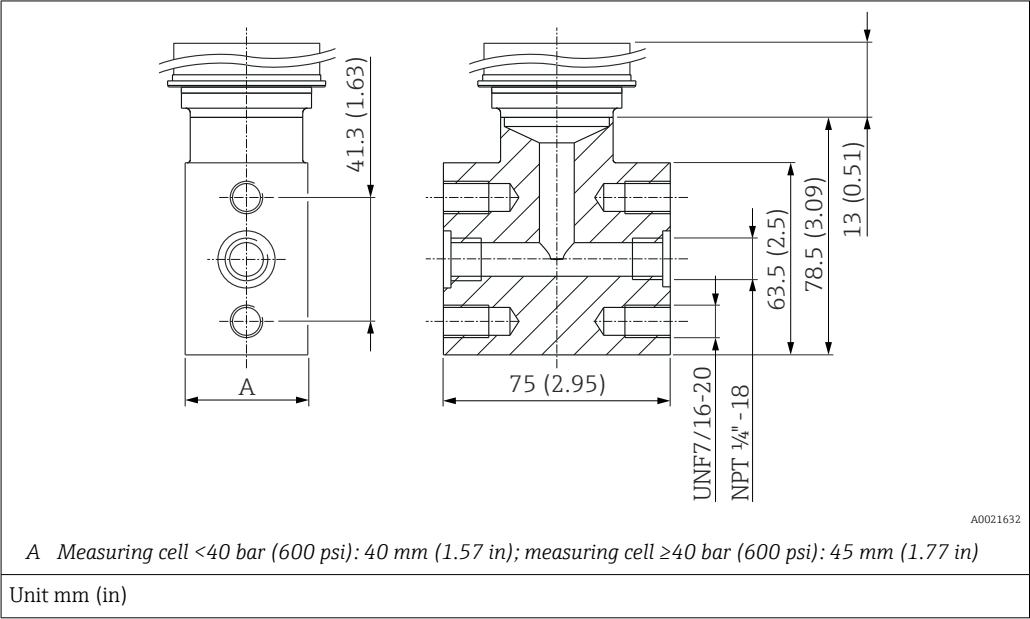

| Material           | Designation                                                                 | Weight     | Option <sup>1)</sup> |
|--------------------|-----------------------------------------------------------------------------|------------|----------------------|
|                    |                                                                             | kg (lb)    |                      |
| AISI 316L (1.4404) | Oval flange adapter 1/4-18 NPT<br>as per IEC 61518<br>Mounting: 7/16-20 UNF | 1.9 (4.19) | UR                   |

1) Product Configurator, order code for "Process connection"

Process connections PMP71      **Prepared for diaphragm seal mounting**

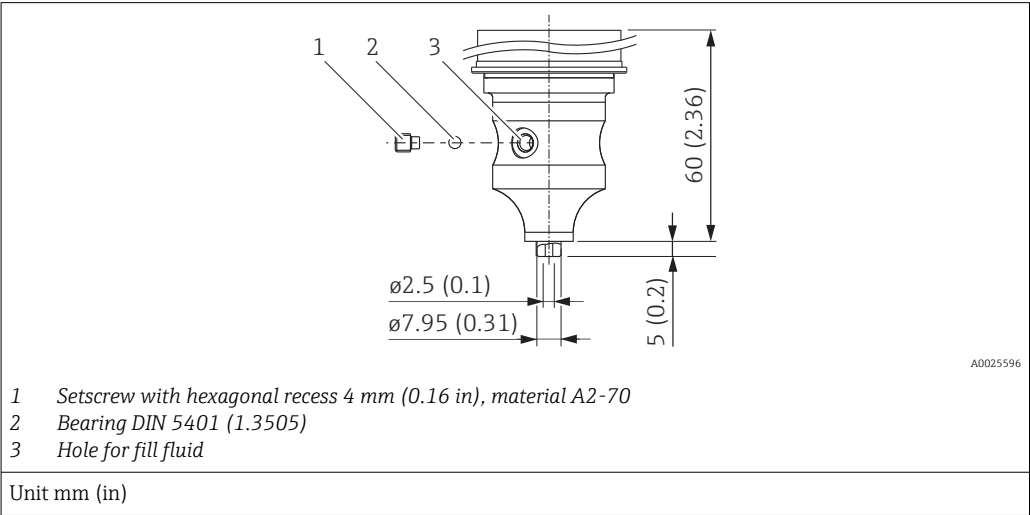


| Material           | Designation                          | Weight kg (lb) | Option <sup>1)</sup> |
|--------------------|--------------------------------------|----------------|----------------------|
| AISI 316L (1.4404) | Prepared for diaphragm seal mounting | 1.9 (4.19)     | U1                   |

1) Product Configurator, order code for "Process connection"

**Valve manifold DA63M-  
(optional)**

Endress+Hauser supplies milled valve manifolds via the transmitter's product structure in the following versions:

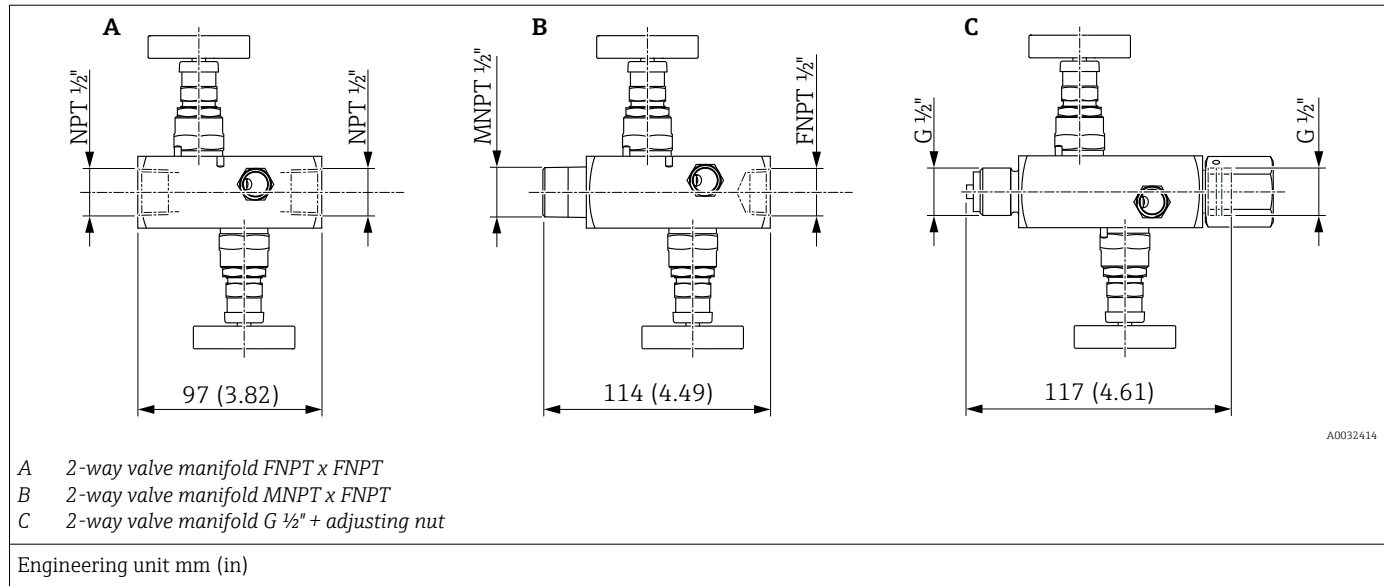


2-way valve manifolds in 316L or AlloyC can be

- ordered as an **enclosed** accessory (seal for mounting is enclosed)
- ordered as a **mounted** accessory (mounted valve manifolds are supplied with a documented leakage test).

Certificates ordered with the equipment (e.g. 3.1 material certificate and NACE) and tests (e.g. PMI and pressure test) apply to the transmitter and the valve manifold.

For other details (order option, dimension, weight, materials), see SD01553P/00/EN "Mechanical accessories for pressure measuring devices".


During the operating life of the valves, it may be necessary to re-tighten the packing.

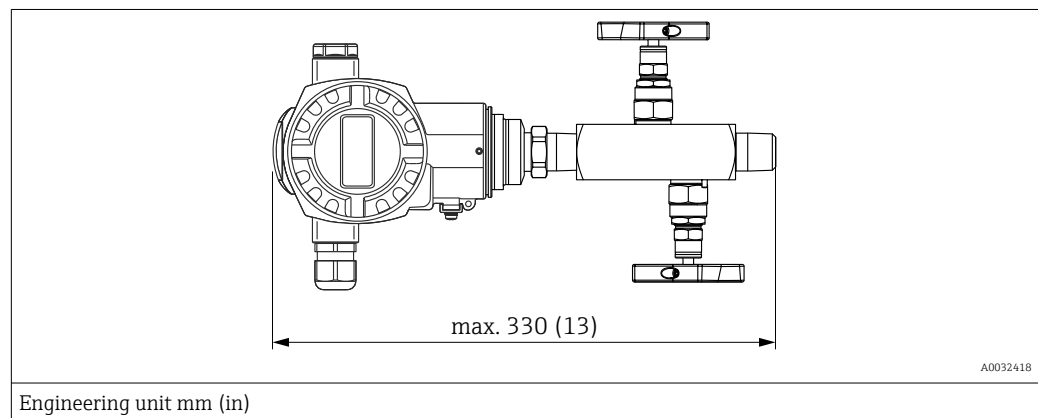**Mounting on valve manifold**

Ordering information:

Product Configurator, order code for "Accessories mounted"

## PMP75 basic device

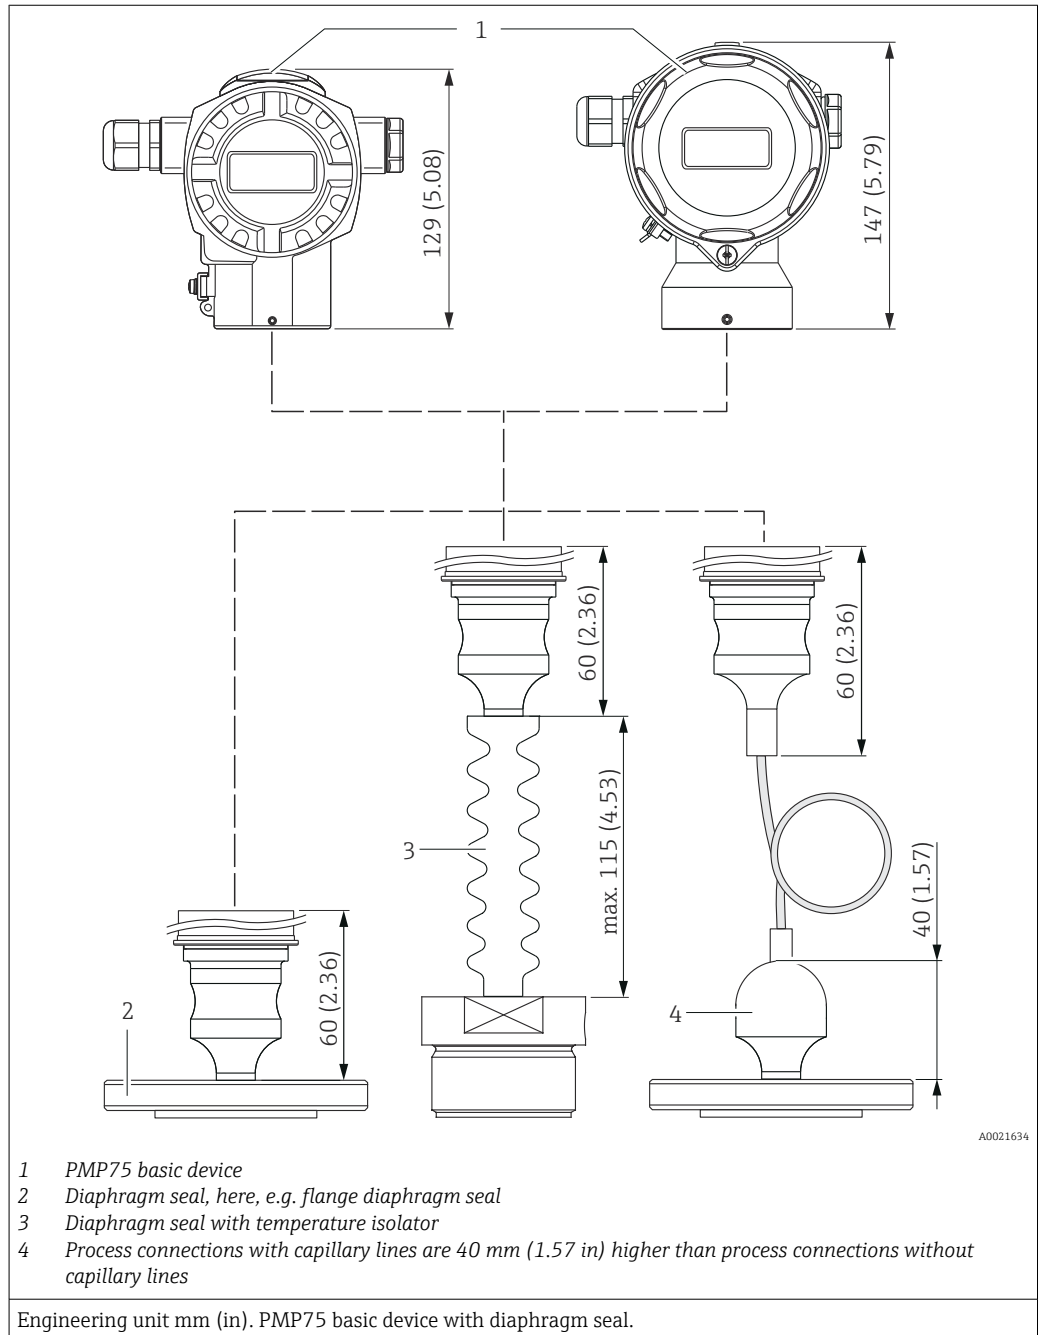


## Process connections PMP75, flush process membrane



- The weights of the diaphragm seals are given in the tables. For the weight of the housing, see → 51
- The following drawings illustrate how the system works in principle. In other words, the dimensions of a diaphragm seal supplied may deviate from the dimensions given in this document.
- Observe the information in the "Planning instructions for diaphragm seal systems" section → 112
- For further information please contact your local Endress+Hauser Sales Center.

## Pancake seal

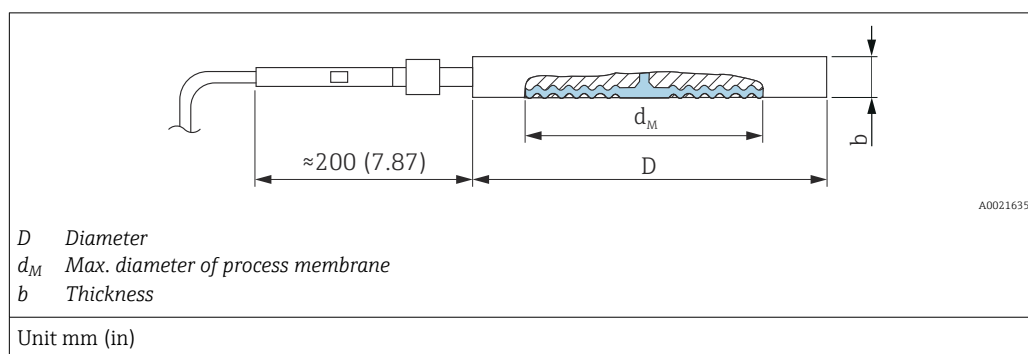

| Flange    |     |        |      |         | Diaphragm seal | Option <sup>1)</sup> |
|-----------|-----|--------|------|---------|----------------|----------------------|
| Material  | DN  | PN     | D    | b       | Weight         |                      |
|           |     |        | [mm] | [mm]    | [kg (lb)]      |                      |
| AISI 316L | 50  | 16-400 | 102  | 20 - 22 | 1.3 (2.87)     | UI <sup>2)</sup>     |
|           | 80  | 16-400 | 138  | 20 - 22 | 2.3 (5.07)     | UJ <sup>2)</sup>     |
|           | 100 | 16-400 | 162  | 20 - 22 | 3.1 (6.84)     | UK                   |

1) Product Configurator, order code for "Process connection"

2) With TempC process membrane

| Flange    |     |          |      |             | Diaphragm seal | Option <sup>1)</sup> |
|-----------|-----|----------|------|-------------|----------------|----------------------|
| Material  | NPS | Class    | D    | b           | Weight         |                      |
|           |     |          | [in] | [in]        | [kg (lb)]      |                      |
| AISI 316L | 2   | 150-2500 | 3.89 | 0.79 - 0.87 | 1.3 (2.87)     | UL <sup>2)</sup>     |
|           | 3   | 150-2500 | 5.00 | 0.79 - 0.87 | 2.3 (5.07)     | UM                   |
|           | 4   | 150-2500 | 6.22 | 0.79 - 0.87 | 3.1 (6.84)     | UR                   |

1) Product Configurator, order code for "Process connection"


2) With TempC process membrane

Maximum diameter of the process membrane  $\varnothing d_M$ 

| DN  | PN     | $\varnothing d_M$ (mm) |      |            |          |                   |      |
|-----|--------|------------------------|------|------------|----------|-------------------|------|
|     |        | 316L TempC             | 316L | Alloy C276 | Tantalum | Monel (Alloy 400) | PTFE |
| 50  | 16-400 | 61                     | 58   | 62         | 60       | 59                | 52   |
| 80  | 16-400 | 89                     | 89   | 90         | 92       | 89                | 80   |
| 100 | 16-400 | -                      | 89   | 90         | 92       | 89                | -    |

| NPS | Class    | $\varnothing d_M$ (in) |      |            |          |                   |      |
|-----|----------|------------------------|------|------------|----------|-------------------|------|
|     |          | 316L TempC             | 316L | Alloy C276 | Tantalum | Monel (Alloy 400) | PTFE |
| 2   | 150-2500 | 2.40                   | 2.05 | 2.32       | 2.36     | 2.32              | 2.05 |
| 3   | 150-2500 | 3.50                   | 3.50 | 3.54       | 3.62     | 3.50              | 3.14 |
| 4   | 150-2500 | -                      | 3.14 | 3.50       | 3.62     | 3.50              | -    |

# Process connections PMP75, ISO 228 and ANSI thread flush process membrane

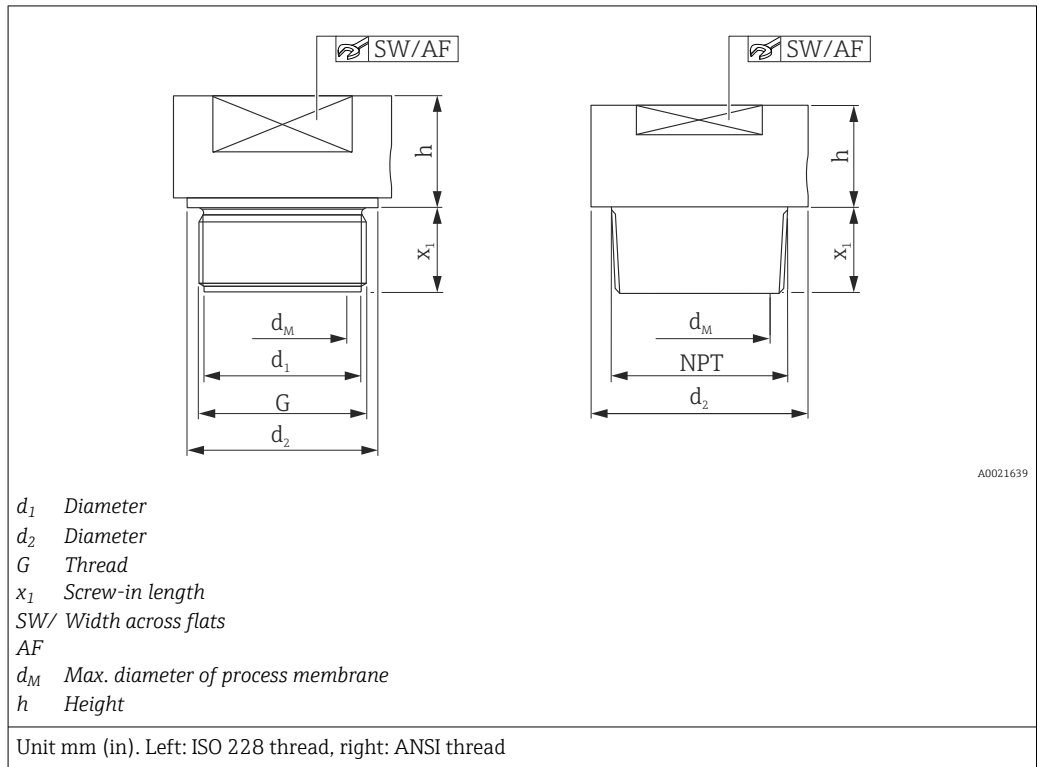


A0021639

| Thread     |           |     |       |       |                  |    | Diaphragm seal |      |            | Option <sup>1)</sup> |
|------------|-----------|-----|-------|-------|------------------|----|----------------|------|------------|----------------------|
| Material   | G         | PN  | $d_1$ | $d_2$ | $x_1$            | AF | $d_M$          | h    | Weight     |                      |
|            |           |     | [mm]  | [mm]  | [mm]             |    | [mm]           | [mm] | [kg (lb)]  |                      |
| AISI 316L  | G 1" A    | 400 | 30    | 39    | 21 <sup>2)</sup> | 32 | 30             | 19   | 0.4 (0.88) | 1D                   |
| Alloy C276 |           |     |       |       |                  |    |                |      | 0.5 (1.1)  | 1E                   |
| AISI 316L  | G 1 ½" A  | 400 | 44    | 55    | 30               | 50 | 42             | 20   | 0.9 (1.98) | 1G                   |
| Alloy C276 |           |     |       |       |                  |    |                |      | 1.0 (2.21) | 1H                   |
| AISI 316L  | G 2"      | 400 | 56    | 68    | 30               | 65 | 50             | 20   | 1.9 (4.19) | 1K                   |
| Alloy C276 |           |     |       |       |                  |    |                |      | 2.1 (4.63) | 1L                   |
| AISI 316L  | 1" MNPT   | 400 | –     | 45    | 28               | 41 | 24             | 17   | 0.6 (1.32) | 2A                   |
| Alloy C276 |           |     |       |       |                  |    |                |      | 0.7 (1.54) | 2B                   |
| AISI 316L  | 1 ½" MNPT | 400 | –     | 60    | 30               | 41 | 36             | 20   | 0.9 (1.98) | 2D                   |
| Alloy C276 |           |     |       | 52    | 30               | 46 | 32             | 20   | 1.0 (2.21) | 2E                   |
| AISI 316L  | 2" MNPT   | 400 | –     | 78    | 30               | 65 | 38             | 25   | 1.8 (3.97) | 2G                   |
| Alloy C276 |           |     |       |       |                  |    |                |      | 2.0 (4.41) | 2H                   |

1) Product Configurator, order code for "Process connection"

2) 28 mm (1.1 in) in conjunction with high-temperature oil

Process connections PMP75, ISO228 and ASME thread, TempC  
flush TempC process  
membrane

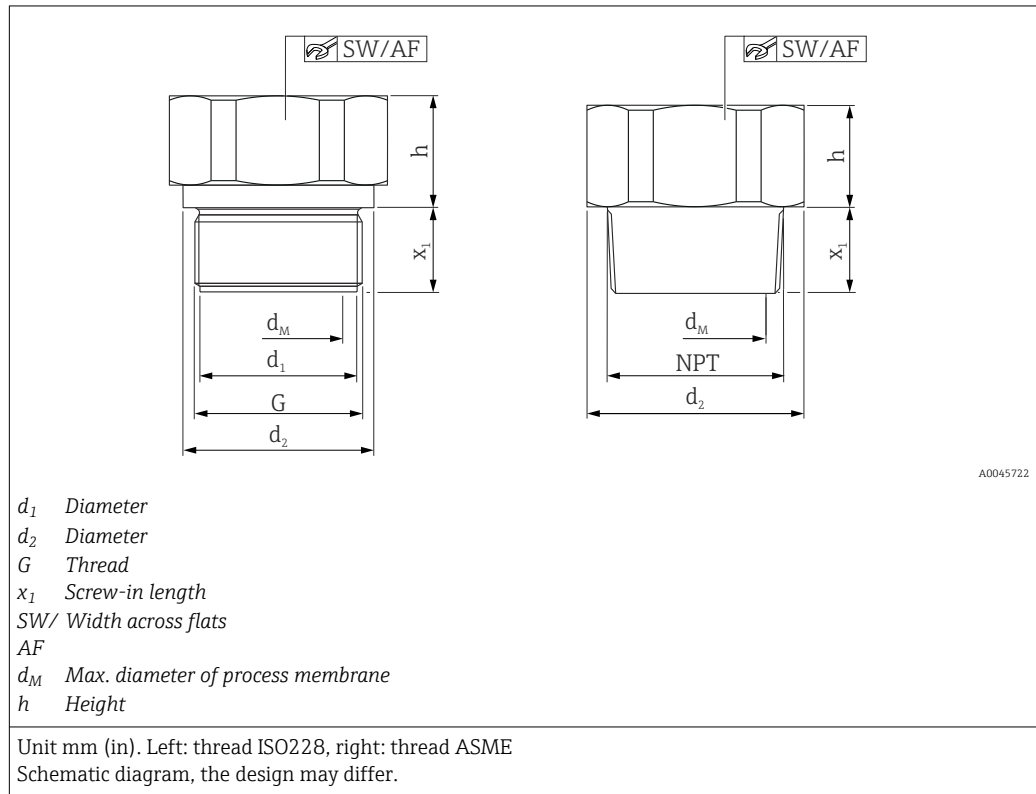


| Thread     |          |     |                      |                      |                      |    | Diaphragm seal       |          |             | Option <sup>1)</sup> |
|------------|----------|-----|----------------------|----------------------|----------------------|----|----------------------|----------|-------------|----------------------|
| Material   | G        | PN  | <i>d<sub>1</sub></i> | <i>d<sub>2</sub></i> | <i>x<sub>1</sub></i> | AF | <i>d<sub>M</sub></i> | <i>h</i> | Weight      |                      |
|            |          |     | [mm]                 | [mm]                 | [mm]                 |    | [mm]                 | [mm]     | [kg (lb)]   |                      |
| AISI 316L  | G 1" A   | 400 | 30                   | 39                   | 21                   | 41 | 28                   | 19       | 0.35 (0.77) | 1D                   |
| Alloy C276 |          |     |                      |                      |                      |    |                      |          | 0.38 (0.84) | 1E                   |
| AISI 316L  | G 1 ½" A | 400 | –                    | 55                   | 30                   | 46 | 41                   | 20       | 0.73 (1.61) | 1G                   |
| Alloy C276 |          |     |                      |                      |                      |    |                      |          | 0.79 (1.74) | 1H                   |
| AISI 316L  | G 2"     | 400 | –                    | 68                   | 30                   | 60 | 48                   | 20       | 1.20 (2.65) | 1K                   |
| Alloy C276 |          |     |                      |                      |                      |    |                      |          | 1.30 (2.87) | 1L                   |

1) Product Configurator, order code for "Process connection"

| Thread     |           |     |                      |                      |                      |    | Diaphragm seal       |          |             | Option <sup>1)</sup> |
|------------|-----------|-----|----------------------|----------------------|----------------------|----|----------------------|----------|-------------|----------------------|
| Material   | MNPT      | PN  | <i>d<sub>1</sub></i> | <i>d<sub>2</sub></i> | <i>x<sub>1</sub></i> | AF | <i>d<sub>M</sub></i> | <i>h</i> | Weight      |                      |
|            |           |     | [mm]                 | [mm]                 | [mm]                 |    | [mm]                 | [mm]     | [kg (lb)]   |                      |
| AISI 316L  | 1" MNPT   | 400 | –                    | 45                   | 23                   | 41 | 28                   | 16       | 0.38 (0.84) | 2A                   |
| Alloy C276 |           |     |                      |                      |                      |    |                      |          | 0.41 (0.90) | 2B                   |
| AISI 316L  | 1 ½" MNPT | 400 | –                    | 60                   | 30                   | 46 | 41                   | 20       | 0.70 (1.54) | 2D                   |
| Alloy C276 |           |     |                      |                      |                      |    |                      |          | 0.76 (1.68) | 2E                   |
| AISI 316L  | 2" MNPT   | 400 | –                    | 60                   | 34                   | 46 | 48                   | 21       | 1.10 (2.43) | 2G                   |
| Alloy C276 |           |     |                      |                      |                      |    |                      |          | 1.19 (2.62) | 2H                   |

1) Product Configurator, order code for "Process connection"

# Process connections PMP75, flush process membrane Tri-Clamp ISO 2852



A0021644

$C_7$  Diameter of flange  
 $h$  Height  
 $d_M$  Max. diameter of process membrane

Unit mm (in)


| Material <sup>1)</sup> | DN<br>ISO 2852 | DN<br>DIN 32676 | NPS | $C_7$ | $d_M$    |       | $h$ | Weight      | Option <sup>2)</sup> |
|------------------------|----------------|-----------------|-----|-------|----------|-------|-----|-------------|----------------------|
|                        |                |                 |     |       | Standard | TempC |     |             |                      |
|                        |                |                 |     |       | [mm]     | [mm]  |     |             |                      |
| AISI 316L              | 25 / 33.7      | 25              | 1   | 50.5  | 24       | -     | 37  | 0.32 (0.71) | TB                   |
|                        | 38             | 40              | 1 ½ | 50.5  | 36       | 36    | 30  | 1 (2.21)    | TC <sup>3) 4)</sup>  |
|                        | 51 / 40        | 50              | 2   | 64    | 48       | 41    | 30  | 1.1 (2.43)  | TD <sup>3) 4)</sup>  |
|                        | 63.5           | 50              | 2 ½ | 77.5  | 61       | 61    | 30  | 0.7 (1.54)  | TE <sup>5)</sup>     |
|                        | 76.1           | -               | 3   | 91    | 73       | 61    | 30  | 1.2 (2.65)  | TF <sup>4)</sup>     |

- 1) Surface roughness of the surfaces in contact with the medium  $R_a < 0.76 \mu\text{m}$  (29.9  $\mu\text{in}$ ) as standard. Lower surface roughness available on request.
- 2) Product Configurator, order code for "Process connection"
- 3) Optionally available as an ASME BPE-compliant diaphragm seal version for use in biochemical processes, surfaces in contact with medium  $R_a < 0.38 \mu\text{m}$  (15  $\mu\text{in}$ ), electropolished; order using order code for "Additional options", option "P".
- 4) Alternatively available with TempC process membrane.
- 5) With TempC process membrane



Max. PN = 40 bar (580 psi). The maximum PN depends on the clamp used.

Process connections PMP75, Tri-Clamp ISO 2852 inline seal  
flush process membrane

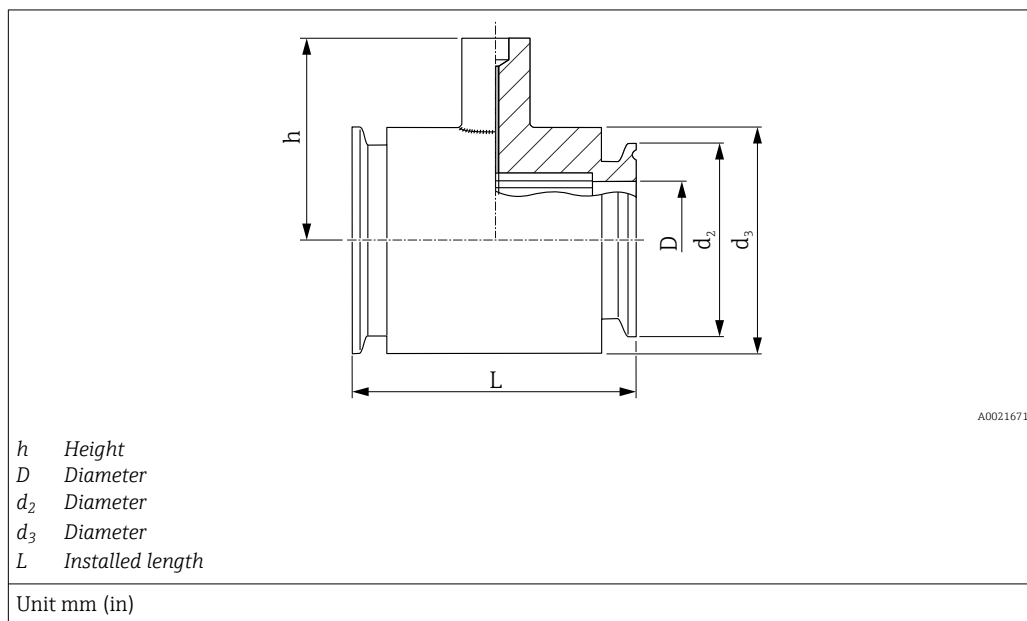


| Material <sup>1)</sup> | DN<br>ISO 2852 | NPS  | PN | D    | d <sub>2</sub> | d <sub>3</sub> | h    | L    | Weight     | Option <sup>2)</sup> |
|------------------------|----------------|------|----|------|----------------|----------------|------|------|------------|----------------------|
|                        |                | [in] |    | [mm] | [mm]           | [mm]           | [mm] | [mm] | [kg (lb)]  |                      |
| AISI 316L              | 25             | 1    | 40 | 22.5 | 50.5           | 54             | 67   | 126  | 1.7 (3.75) | SB                   |
|                        | 38             | 1 ½  | 40 | 35.5 | 50.5           | 69             | 67   | 126  | 1.0 (2.21) | SC <sup>3)</sup>     |
|                        | 51             | 2    | 40 | 48.6 | 64             | 78             | 79   | 100  | 1.7 (3.75) | SD <sup>3)</sup>     |

1) Surface roughness of the surfaces in contact with the medium  $R_a < 0.76 \mu\text{m}$  (29.9  $\mu\text{in}$ ) as standard.

2) Product Configurator, order code for "Process connection"

3) incl. 3.1 and pressure test according to Pressure Equipment Directive, Category II


**Hygienic process connections**    **Varivent for pipes**  
**PMP75, flush process**  
**membrane**

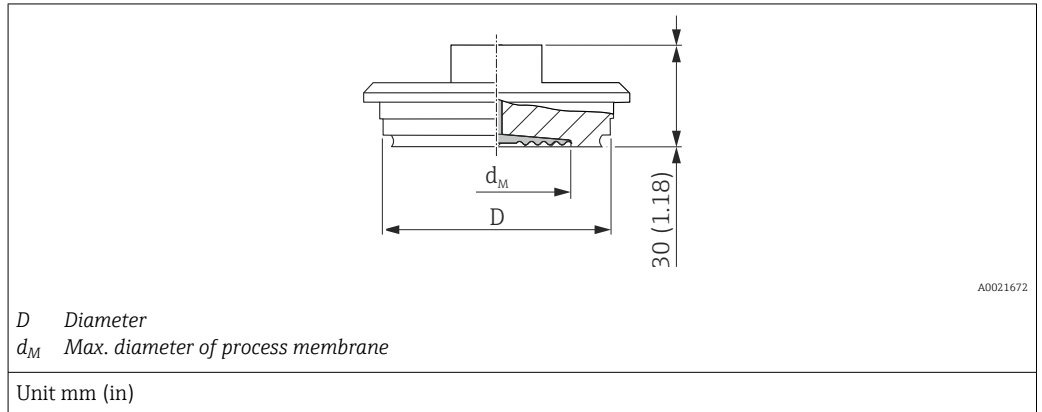

| Material <sup>1)</sup> | Designation      | DN       | PN | D  | $d_M$    |       | Weight     | Option <sup>2)</sup> |
|------------------------|------------------|----------|----|----|----------|-------|------------|----------------------|
|                        |                  |          |    |    | Standard | TempC |            |                      |
|                        |                  |          |    |    | [mm]     | [mm]  |            |                      |
| AISI 316L              | Type F for pipes | 25 - 32  | 40 | 50 | 34       | 36    | 0.4 (0.88) | TU <sup>3)</sup>     |
| AISI 316L              | Type N for pipes | 40 - 162 | 40 | 68 | 58       | 61    | 0.8 (1.76) | TR <sup>4) 5)</sup>  |

- 1) Roughness of surfaces in contact with the medium  $R_a < 0.76 \mu\text{m}$  ( $29.9 \mu\text{in}$ ) as standard.
- 2) Product Configurator, order code for "Process connection"
- 3) With TempC process membrane
- 4) Optionally available as an ASME BPE-compliant diaphragm seal version for use in biochemical processes, surfaces in contact with medium  $R_a < 0.38 \mu\text{m}$  ( $15 \mu\text{in}$ ), electropolished; order using order code for "Additional options", option "P". Lower surface roughness on request.
- 5) Alternatively available with TempC process membrane.


**DRD DN50 (65 mm)**

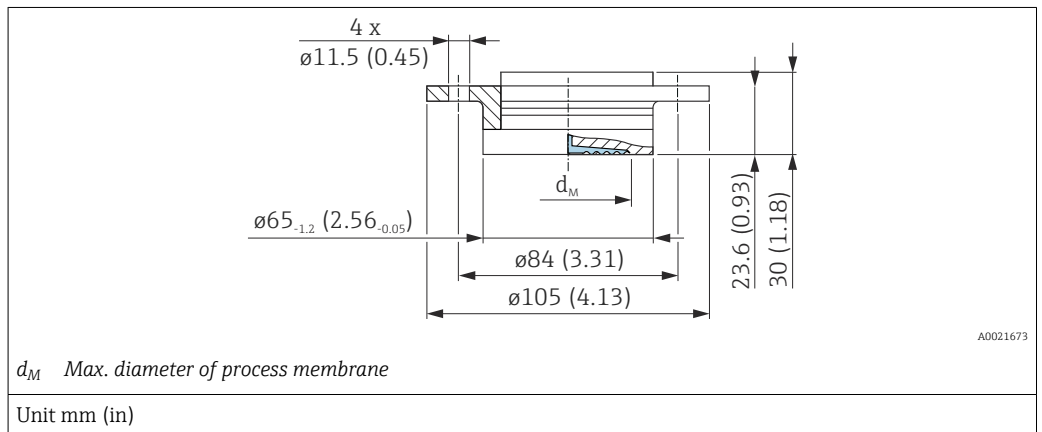

| Material <sup>1)</sup> | PN | $d_M$    |       | Weight      | Option <sup>2)</sup> |
|------------------------|----|----------|-------|-------------|----------------------|
|                        |    | Standard | TempC |             |                      |
|                        |    | [mm]     | [mm]  |             |                      |
| AISI 316L              | 25 | 50       | 48    | 0.75 (1.65) | TK <sup>3) 4)</sup>  |

- 1) Surface roughness of the surfaces in contact with the medium  $R_a < 0.76 \mu\text{m}$  ( $29.9 \mu\text{in}$ ) as standard.
- 2) Product Configurator, order code for "Process connection"
- 3) Alternatively available with TempC process membrane.
- 4) Including slip-on flange.

Hygienic process connections    SMS nozzle with coupling nut  
PMP75, flush process  
membrane

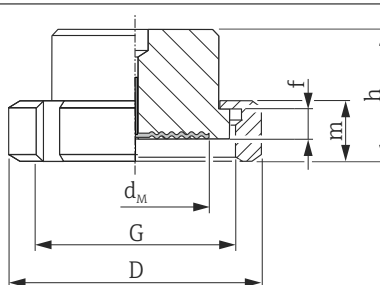

A0021674

*D*    Diameter  
*f*    Nozzle height  
*G*    Thread  
*h*    Height  
*m*    Height  
*d<sub>M</sub>*    Max. diameter of process membrane

Unit mm (in)


| Material <sup>1)</sup> | NPS | PN | D    | f    | G           | m    | h    | d <sub>M</sub> | Weight<br>[kg (lb)] | Option <sup>2)</sup> |
|------------------------|-----|----|------|------|-------------|------|------|----------------|---------------------|----------------------|
|                        |     |    | [mm] | [mm] |             | [mm] | [mm] | [mm]           |                     |                      |
| AISI 316L              | 1   | 25 | 54   | 3.5  | Rd 40 – 1/6 | 20   | 42.5 | 24             | 0.25 (0.55)         | TG                   |
|                        | 1 ½ | 25 | 74   | 4    | Rd 60 – 1/6 | 25   | 57   | 36             | 0.65 (1.43)         | TH <sup>3)</sup>     |
|                        | 2   | 25 | 84   | 4    | Rd 70 – 1/6 | 26   | 62   | 48             | 1.05 (2.32)         | TI <sup>3)</sup>     |

1) Roughness of surfaces in contact with the medium  $R_a < 0.76 \mu\text{m}$  ( $29.9 \mu\text{in}$ ) as standard.

2) Product Configurator, order code for "Process connection"

3) Alternatively available with TempC process membrane.


Hygienic process connections Taper adapter with grooved union nut, DIN 11851  
PMP75, flush process membrane

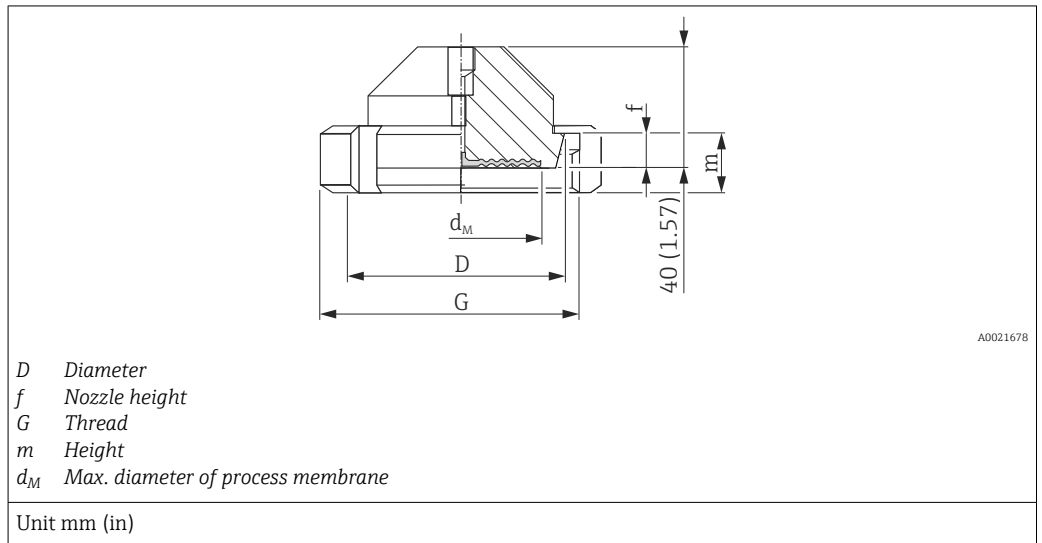

| Material <sup>1)</sup> | Taper adapter |       |      |      | Slotted nut   |      | Diaphragm seal |       |             | Option <sup>2)</sup> |
|------------------------|---------------|-------|------|------|---------------|------|----------------|-------|-------------|----------------------|
|                        |               |       |      |      |               |      | d <sub>M</sub> |       | Weight      |                      |
|                        | DN            | PN    | D    | f    | G             | m    | Standard       | TempC | [kg (lb)]   |                      |
|                        |               | [bar] | [mm] | [mm] |               | [mm] | [mm]           | [mm]  |             |                      |
| AISI 316L              | 32            | 40    | 50   | 10   | Rd 58 x 1/6"  | 21   | 32             | 28    | 0.45 (0.99) | MI <sup>3)</sup>     |
|                        | 40            | 40    | 56   | 10   | Rd 65 x 1/6"  | 21   | 38             | 36    | 0.45 (0.99) | MZ <sup>3)</sup>     |
|                        | 50            | 25    | 68.5 | 11   | Rd 78 x 1/6"  | 19   | 52             | 48    | 1.1 (2.43)  | MR <sup>4)</sup>     |
|                        | 65            | 25    | 86   | 12   | Rd 95 x 1/6"  | 21   | 66             | 61    | 2.0 (4.41)  | MS <sup>4)</sup>     |
|                        | 80            | 25    | 100  | 12   | Rd 110 x 1/4" | 26   | 81             | 61    | 2.55 (5.62) | MT <sup>4)</sup>     |

- 1) Roughness of wetted surfaces  $R_a < 0.76 \mu\text{m}$  (29.9  $\mu\text{in}$ ) as standard.
- 2) Product Configurator, order code for "Process connection"
- 3) With TempC process membrane
- 4) Alternatively available with TempC process membrane.

# NEUMO BioControl

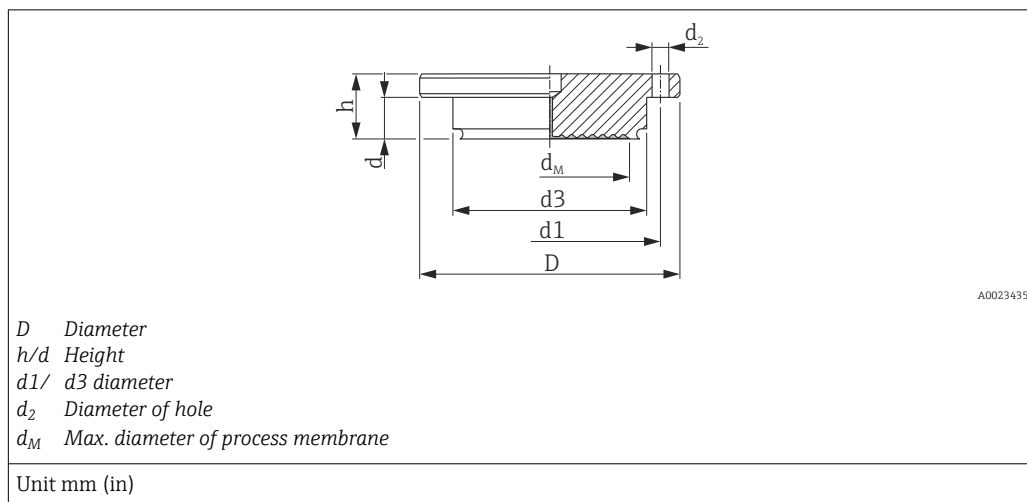

| Material <sup>1)</sup> | NEUMO BioControl <sup>2)</sup> |       |      |      |                |                |                |      | Diaphragm seal |       |            | Option <sup>3)</sup> |
|------------------------|--------------------------------|-------|------|------|----------------|----------------|----------------|------|----------------|-------|------------|----------------------|
|                        |                                |       |      |      |                |                |                |      | d <sub>M</sub> |       | Weight     |                      |
|                        | DN                             | PN    | D    | d    | d <sub>2</sub> | d <sub>3</sub> | d <sub>1</sub> | m    | Standard       | TempC |            |                      |
|                        |                                | [bar] | [mm] | [mm] | [mm]           | [mm]           | [mm]           | [mm] | [mm]           | [mm]  | [kg (lb)]  |                      |
| AISI 316L              | 50                             | 16    | 90   | 17   | 4 x Ø 9        | 50             | 70             | 27   | 40             | 36    | 1.1 (2.43) | S4 <sup>4)</sup>     |
|                        | 80                             | 16    | 140  | 25   | 4 x Ø 11       | 87.4           | 115            | 37   | 61             | 61    | 2.6 (5.73) | S6 <sup>4)</sup>     |


1) Surface roughness of the surfaces in contact with the medium  $R_a < 0.76 \mu\text{m}$  (29.9  $\mu\text{in}$ ) as standard.

2) (Process temperature range: -10 to +200 °C (+14 to +392 °F))

3) Product Configurator, order code for "Process connection"

4) With TempC process membrane

Universal process adapter

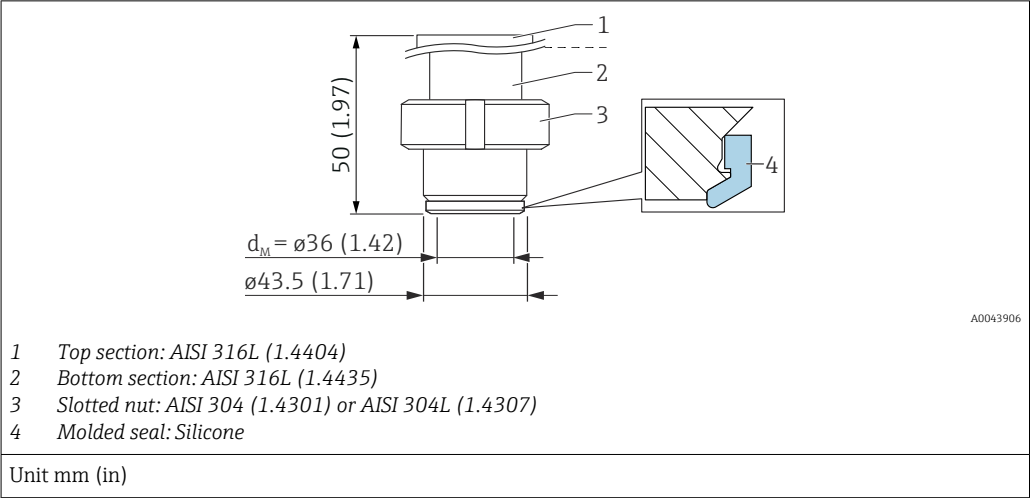


- The roughness of the surface in contact with the medium  $R_a < 0.76 \mu\text{m}$  (30  $\mu\text{in}$ )
- Temperature operating range:  $-60$  to  $+150^\circ\text{C}$  ( $-76$  to  $+302^\circ\text{F}$ )
- Silicone form seal: FDA 21CFR177.2600/USP Class VI, order number: 52023572

| Designation                                         | PN        | Weight     | Option <sup>1)</sup> |
|-----------------------------------------------------|-----------|------------|----------------------|
|                                                     | bar (psi) | [kg (lb)]  |                      |
| Universal process adapter<br>Silicone form seal (4) | 10        | 0.8 (1.76) | 00 <sup>2)</sup>     |

1) Product Configurator, order code for "Process connection"

2) Alternatively available with TempC process membrane.

**Process connections PMP75, EN flanges, connection dimensions as per EN 1092-1**  
**flush process membrane**

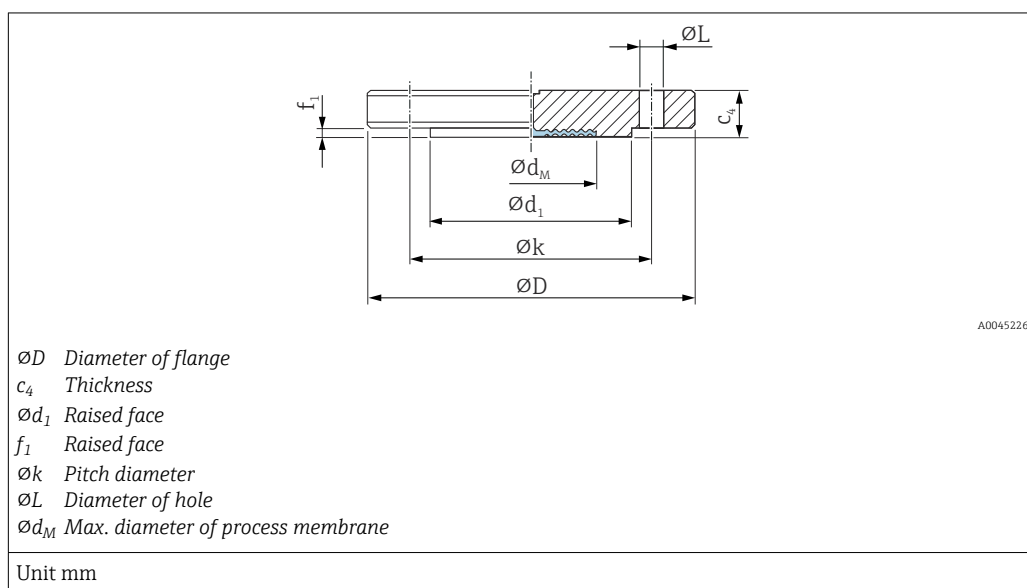

| Flange <sup>1) 2) 3)</sup> |            |      |                 |       |                   |       | Boltholes |                 |                 | Diaphragm seal | Option <sup>4)</sup> |
|----------------------------|------------|------|-----------------|-------|-------------------|-------|-----------|-----------------|-----------------|----------------|----------------------|
| DN                         | PN         | Form | $\varnothing D$ | $c_4$ | $\varnothing d_1$ | $f_1$ | Quantity  | $\varnothing L$ | $\varnothing k$ | Weight         |                      |
|                            |            |      | mm              | mm    | mm                | mm    |           | mm              | mm              | kg (lb)        |                      |
| DN 25                      | PN 10-40   | B1   | 115             | 18    | 68                | 2     | 4         | 14              | 85              | 1.38 (3.04)    | CN <sup>5) 6)</sup>  |
| DN 25                      | PN 63-160  | B2   | 140             | 24    | 68                | 2     | 4         | 18              | 100             | 2.54 (5.60)    | DN                   |
| DN 25                      | PN 250     | B2   | 150             | 28    | 68                | 2     | 4         | 22              | 105             | 3.7 (8.16)     | EN                   |
| DN 25                      | PN 400     | B2   | 180             | 38    | 68                | 2     | 4         | 26              | 130             | 6.65 (14.66)   | E1                   |
| DN 32                      | PN 10-40   | B1   | 140             | 18    | 78                | 2     | 4         | 18              | 100             | 2.03 (4.48)    | CP                   |
| DN 40                      | PN 10-40   | B1   | 150             | 18    | 88                | 3     | 4         | 18              | 110             | 2.35 (5.18)    | CQ                   |
| DN 50                      | PN 10-40   | B1   | 165             | 20    | 102               | 3     | 4         | 18              | 125             | 3.2 (7.06)     | B3 <sup>5) 6)</sup>  |
| DN 50                      | PN 63      | B2   | 180             | 26    | 102               | 3     | 4         | 22              | 135             | 4.52 (9.97)    | C3                   |
| DN 50                      | PN 100-160 | B2   | 195             | 30    | 102               | 3     | 4         | 26              | 145             | 6.07 (13.38)   | EF                   |
| DN 50                      | PN 250     | B2   | 200             | 38    | 102               | 3     | 8         | 26              | 150             | 7.7 (16.98)    | ER                   |
| DN 50                      | PN 400     | B2   | 235             | 52    | 102               | 3     | 8         | 30              | 180             | 14.7 (32.41)   | E3                   |
| DN 80                      | PN 10-40   | B1   | 200             | 24    | 138               | 3     | 8         | 18              | 160             | 5.54 (12.22)   | B4 <sup>5) 6)</sup>  |
| DN 80                      | PN 100     | B2   | 230             | 32    | 138               | 3     | 8         | 26              | 180             | 8.85 (19.51)   | C4                   |
| DN 100                     | PN 100     | B2   | 265             | 36    | 162               | 3     | 8         | 30              | 210             | 13.3 (29.33)   | C5                   |

1) Material: AISI 316L

2) The roughness of the surface in contact with the medium including the raised face of the flanges (all standards) made of Alloy C276, Monel, tantalum, gold > 316L or PTFE is  $R_a < 0.8 \mu\text{m}$  (31.5  $\mu\text{in}$ ). Lower surface roughness available on request.

3) The flange raised face is made of the same material as the process membrane.

4) Product Configurator, order code for "Process connection"


5) Alternatively available with TempC process membrane. Change in diameter of process membrane in TempC version: DN25: 28 mm; DN50: 61 mm.

6) Alternatively available with gold-coated TempC process membrane (Product Configurator, order code for "Membrane material" option "G").

Maximum diameter of the process membrane  $\varnothing d_M$

| DN     | PN         | $\varnothing d_M$ (mm) |      |            |          |                      |      |
|--------|------------|------------------------|------|------------|----------|----------------------|------|
|        |            | 316L TempC             | 316L | Alloy C276 | Tantalum | Monel<br>(Alloy 400) | PTFE |
| DN 25  | PN 10-40   | 28                     | 29.6 | 33         | 33       | 33                   | 28   |
| DN 25  | PN 63-160  | -                      | 28   | 28         | 28       | 28                   | -    |
| DN 25  | PN 250     | -                      | 28   | 28         | 28       | 28                   | -    |
| DN 25  | PN 400     | -                      | 28   | 28         | 28       | 28                   | -    |
| DN 32  | PN 10-40   | -                      | 34   | 42         | 42       | 34                   | -    |
| DN 40  | PN 10-40   | -                      | 38   | 48         | 51       | 42                   | -    |
| 50     | PN 10-40   | 61                     | 58   | 57         | 60       | 59                   | 52   |
| DN 50  | PN 63      | -                      | 52   | 62         | 60       | 59                   | -    |
| DN 50  | PN 100-160 | -                      | 52   | 62         | 60       | 59                   | -    |
| DN 50  | PN 250     | -                      | 52   | 62         | 60       | 59                   | -    |
| DN 50  | PN 400     | -                      | 52   | 62         | 60       | 59                   | -    |
| DN 80  | PN 10-40   | 89                     | 89   | 89         | 92       | 89                   | 80   |
| DN 80  | PN 100     | -                      | 80   | 90         | 92       | 90                   | -    |
| DN 100 | PN 100     | -                      | 80   | 90         | 92       | 89                   | -    |

## EN flanges with barrel, connection dimensions as per EN 1092-1

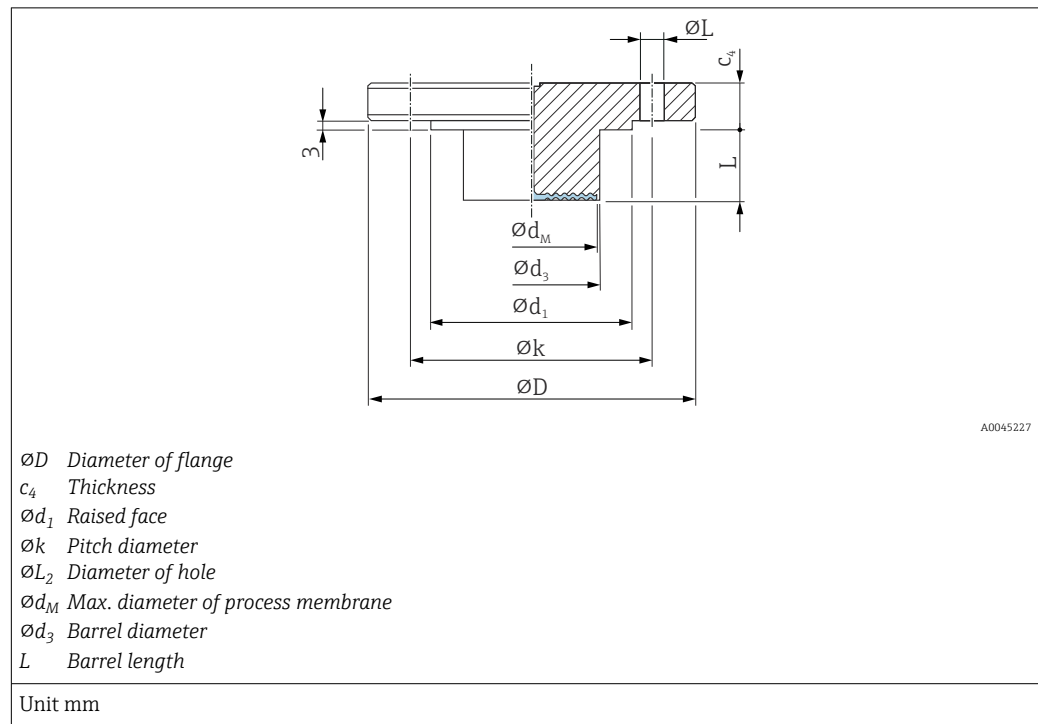

| Flange <sup>1) 2)</sup> |       |      |                 |       |                   | Boltholes |                 |                 | Diaphragm seal |               | Option <sup>3)</sup> |
|-------------------------|-------|------|-----------------|-------|-------------------|-----------|-----------------|-----------------|----------------|---------------|----------------------|
| DN                      | PN    | Form | $\varnothing D$ | $c_4$ | $\varnothing d_1$ | Quantity  | $\varnothing L$ | $\varnothing k$ | $d_M$          | Weight        |                      |
|                         |       |      | mm              | mm    | mm                |           | mm              | mm              | mm             | kg (lb)       |                      |
| 50                      | 10-40 | B1   | 165             | 20    | 102               | 4         | 18              | 125             | 48             | <sup>4)</sup> | D3 <sup>4)</sup>     |
| 80                      | 10-40 | B1   | 200             | 24    | 138               | 8         | 18              | 160             | 73             | <sup>4)</sup> | D4 <sup>4)</sup>     |

1) Material: AISI 316L


2) In the case of process membranes made of Alloy C276, Monel or tantalum, the raised face of the flange and the barrel pipe are made of 316L

3) Product Configurator, order code for "Process connection"

4) Available with 50 mm (1.97 in), 100 mm (3.94 in) and 200 mm (7.87 in) barrel (extended diaphragm seal), for barrel diameter and weight, see the following table

| Option <sup>1)</sup> | DN | PN    | L              | $d_3$ | Weight                                              |
|----------------------|----|-------|----------------|-------|-----------------------------------------------------|
|                      |    |       | [mm]           | [mm]  | [kg (lb)]                                           |
| D3                   | 50 | 10-40 | 50 / 100 / 200 | 48.3  | 3.44 (7.59) / 3.8 (8.4) / 4.1 (9.04) / 4.4 (9.7)    |
| D4                   | 80 | 10-40 | 50 / 100 / 200 | 76    | 6.2 (13.7) / 6.7 (14.8) / 7.27 (16.03) / 7.8 (17.2) |

1) Product Configurator, order code for "Process connection"

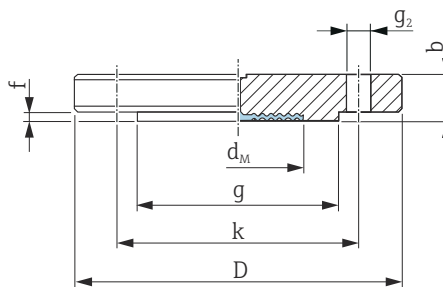**Process connections PMP75,  
flush process membrane**
**ASME flanges, connection dimensions as per ASME B 16.5, raised face RF**


A0023913

*D* Diameter of flange  
*b* Thickness  
*g* Raised face  
*f* Raised face  
*k* Pitch diameter  
*g<sub>2</sub>* Diameter of hole  
*d<sub>M</sub>* Max. diameter of process membrane

Unit in


| Flange <sup>1) 2) 3)</sup> |             |      |      |      |      | Boltholes |                |      | Diaphragm seal | Option <sup>4)</sup> |
|----------------------------|-------------|------|------|------|------|-----------|----------------|------|----------------|----------------------|
| NPS                        | Class       | D    | b    | g    | f    | Quantity  | g <sub>2</sub> | k    | Weight         |                      |
| [in]                       | [lb./sq.in] | [in] | [in] | [in] | [in] |           | [in]           | [in] | [kg (lb)]      |                      |
| 1                          | 150         | 4.25 | 0.56 | 2    | 0.08 | 4         | 0.62           | 3.12 | 1.2 (2.65)     | AC <sup>5) 6)</sup>  |
| 1                          | 300         | 4.88 | 0.69 | 2    | 0.08 | 4         | 0.75           | 3.5  | 1.3 (2.87)     | AN <sup>5) 6)</sup>  |
| 1                          | 400/600     | 4.88 | 0.69 | 2    | 0.25 | 4         | 0.75           | 3.5  | 1.4 (3.09)     | HC                   |
| 1                          | 900/1500    | 5.88 | 1.12 | 2    | 0.25 | 4         | 1              | 4    | 3.2 (7.06)     | HN                   |
| 1                          | 2500        | 6.25 | 1.38 | 2    | 0.25 | 4         | 1              | 4.25 | 4.6 (10.14)    | HO                   |
| 1 ½                        | 150         | 5    | 0.69 | 2.88 | 0.06 | 4         | 0.62           | 3.88 | 1.5 (3.31)     | AE                   |
| 1 ½                        | 300         | 6.12 | 0.81 | 2.88 | 0.06 | 4         | 0.88           | 4.5  | 2.6 (5.73)     | AQ                   |
| 2                          | 150         | 6    | 0.75 | 3.62 | 0.06 | 4         | 0.75           | 4.75 | 2.2 (4.85)     | AF <sup>5) 6)</sup>  |
| 2                          | 300         | 6.5  | 0.88 | 3.62 | 0.06 | 8         | 0.75           | 5    | 3.4 (7.5)      | AR <sup>5) 6)</sup>  |
| 2                          | 400/600     | 6.5  | 1    | 3.62 | 0.25 | 8         | 0.75           | 5    | 4.3 (9.48)     | HF                   |
| 2                          | 900/1500    | 8.5  | 1.5  | 3.62 | 0.25 | 8         | 1              | 6.5  | 10.3 (22.71)   | HR                   |
| 2                          | 2500        | 9.25 | 2    | 3.62 | 0.25 | 8         | 1.12           | 6.75 | 15.8 (34.84)   | H3                   |
| 3                          | 150         | 7.5  | 0.94 | 5    | 0.06 | 4         | 0.75           | 6    | 5.1 (11.25)    | AG <sup>5) 6)</sup>  |
| 3                          | 300         | 8.25 | 1.12 | 5    | 0.06 | 8         | 0.75           | 6    | 7.0 (15.44)    | AS <sup>5) 6)</sup>  |
| 4                          | 150         | 9    | 0.94 | 6.19 | 0.06 | 8         | 0.75           | 7.5  | 7.2 (15.88)    | AH                   |
| 4                          | 300         | 10   | 1.25 | 6.19 | 0.06 | 8         | 0.88           | 7.88 | 11.7 (25.8)    | AT                   |

- 1) Material AISI 316/316L: Combination of AISI 316 for required pressure resistance and AISI 316L for required chemical resistance (dual-rated)
- 2) The roughness of the surface in contact with the medium, including the raised face of the flanges (all standards) made of Alloy C276, Monel, tantalum, gold or PTFE, is  $R_a < 0.8 \mu\text{m}$  (31.5  $\mu\text{in}$ ). Lower surface roughness available on request.
- 3) The flange raised face is made of the same material as the process membrane.
- 4) Product Configurator, order code for "Process connection"
- 5) Alternatively available with TempC process membrane. Change in diameter of process membrane in TempC version: nominal diameter 1": 1.1 in; 2": 2.40 in.
- 6) Alternatively available with gold-coated TempC process membrane (Product Configurator, order code for "Membrane material" option "G").

Maximum diameter of the process membrane  $\varnothing d_M$

| NPS | Class    | $\varnothing d_M$ (in) |      |            |          |                      |
|-----|----------|------------------------|------|------------|----------|----------------------|
|     |          | 316L TempC             | 316L | Alloy C276 | Tantalum | Monel<br>(Alloy 400) |
| 1   | 150      | 1.10                   | -    | 1.30       | 1.34     | 1.30                 |
| 1   | 300      | 1.10                   | -    | 1.30       | 1.34     | 1.30                 |
| 1   | 400/600  | -                      | 1.10 | 1.30       | 1.34     | 1.30                 |
| 1   | 900/1500 | -                      | 1.10 | 1.10       | 1.02     | 1.10                 |
| 1   | 2500     | -                      | 1.10 | 1.30       | 1.34     | 1.30                 |
| 1 ½ | 150      | -                      | 1.50 | 1.89       | 2.01     | 1.89                 |
| 1 ½ | 300      | -                      | 1.50 | 1.89       | 2.01     | 1.89                 |
| 2   | 150      | 2.40                   | -    | 2.44       | 2.44     | 2.44                 |
| 2   | 300      | 2.40                   | -    | 2.44       | 2.44     | 2.44                 |
| 2   | 400/600  | -                      | 2.05 | 2.44       | 2.44     | 2.44                 |
| 2   | 900/1500 | -                      | 2.05 | 2.44       | 2.44     | 2.44                 |
| 2   | 2500     | -                      | 2.05 | 2.44       | 2.44     | 2.44                 |
| 3   | 150      | 3.50                   | -    | 3.62       | 3.62     | 3.62                 |
| 3   | 300      | 3.50                   | -    | 3.62       | 3.62     | 3.62                 |
| 4   | 150      | -                      | 3.15 | 3.62       | 3.62     | 3.62                 |
| 4   | 300      | -                      | 3.15 | 3.62       | 3.62     | 3.62                 |

**ASME flanges with barrel (extended diaphragm seal), connection dimensions in accordance with ASME B 16.5, raised face RF**

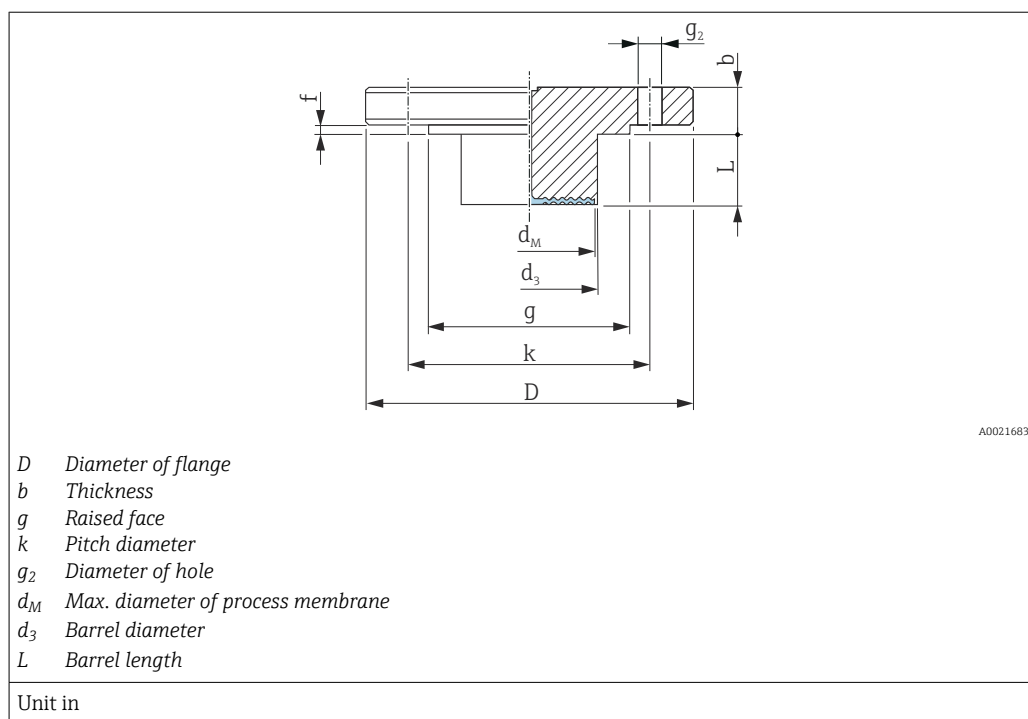


| Flange <sup>1) 2)</sup> |             |      |      |      |      | Boltholes |                      |          | Diaphragm seal       |               | Option <sup>3)</sup> |
|-------------------------|-------------|------|------|------|------|-----------|----------------------|----------|----------------------|---------------|----------------------|
| NPS                     | Class       | D    | b    | g    | f    | Quantity  | <i>g<sub>2</sub></i> | <i>k</i> | <i>d<sub>M</sub></i> | Weight        |                      |
| [in]                    | [lb./sq.in] | [in] | [in] | [in] | [in] |           | [in]                 | [in]     | [in]                 | [kg (lb)]     |                      |
| 2                       | 150         | 6    | 0.75 | 3.62 | 0.06 | 4         | 0.75                 | 4.75     | 1.85                 | <sup>4)</sup> | J3 <sup>4)</sup>     |
| 3                       | 150         | 7.5  | 0.94 | 5    | 0.06 | 4         | 0.75                 | 6        | 2.83                 | <sup>4)</sup> | J4 <sup>4)</sup>     |
| 3                       | 300         | 8.25 | 1.12 | 5    | 0.06 | 8         | 0.88                 | 6.62     | 2.83                 | <sup>4)</sup> | J7 <sup>4)</sup>     |
| 4                       | 150         | 9    | 0.94 | 6.19 | 0.06 | 8         | 0.75                 | 7.5      | 3.5                  | <sup>4)</sup> | J5 <sup>4)</sup>     |
| 4                       | 300         | 10   | 1.25 | 6.19 | 0.06 | 8         | 0.88                 | 7.88     | 3.5                  | <sup>4)</sup> | J8 <sup>4)</sup>     |

- 1) Material: AISI 316/316L. Combination of AISI 316 for required pressure resistance and AISI 316L for required chemical resistance (dual rated)  
2) In the case of process membranes made of Alloy C276, Monel or tantalum, the raised face of the flange and the barrel pipe are made of 316L.  
3) Product Configurator, order code for "Process connection"  
4) Choice of 2", 4", 6" or 8" barrel (extended diaphragm seal), for diameter and weight of barrel (extended diaphragm seal) see the following table

| Option <sup>1)</sup> | NPS  | Class       | (L)                                          | <i>d<sub>3</sub></i> | Weight                                                |
|----------------------|------|-------------|----------------------------------------------|----------------------|-------------------------------------------------------|
|                      | [in] | [lb./sq.in] | in (mm)                                      | in (mm)              | [kg (lb)]                                             |
| J3                   | 2    | 150         | 2 (50.8) / 4 (101.6) / 6 (152.4) / 8 (203.2) | 1.9 (48.3)           | 3.0 (6.6) / 3.4 (7.5) / 3.9 (8.6) / 4.4 (9.7)         |
| J4                   | 3    | 150         | 2 (50.8) / 4 (101.6) / 6 (152.4) / 8 (203.2) | 2.99 (76)            | 6.0 (13.2) / 6.6 (14.5) / 7.1 (15.7) / 7.8 (17.2)     |
| J7                   | 3    | 300         | 2 (50.8) / 4 (101.6) / 6 (152.4) / 8 (203.2) | 2.99 (76)            | 7.9 (17.4) / 8.5 (18.7) / 9.0 (19.9) / 9.6 (21.2)     |
| J5                   | 4    | 150         | 2 (50.8) / 4 (101.6) / 6 (152.4) / 8 (203.2) | 3.7 (94)             | 8.6 (19) / 9.9 (21.8) / 11.2 (24.7) / 12.4 (27.3)     |
| J8                   | 4    | 300         | 2 (50.8) / 4 (101.6) / 6 (152.4) / 8 (203.2) | 3.7 (94)             | 13.1 (28.9) / 14.4 (31.6) / 15.7 (34.6) / 16.9 (37.3) |

- 1) Product Configurator, order code for "Process connection"

## JIS flanges, connection dimensions in accordance with JIS B 2220 BL, raised face RF

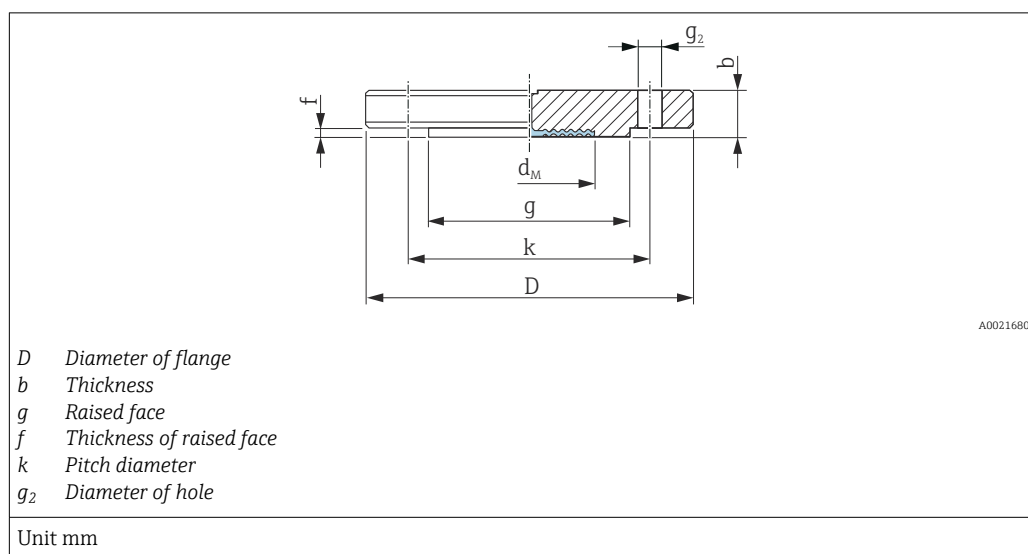

| Flange <sup>1) 2) 3)</sup> |    |      |      |      |      | Boltholes |                |      | Diaphragm seal | Option <sup>4)</sup> |
|----------------------------|----|------|------|------|------|-----------|----------------|------|----------------|----------------------|
| A                          | K  | D    | b    | g    | f    | Quantity  | g <sub>2</sub> | k    | Weight         |                      |
|                            |    | [mm] | [mm] | [mm] | [mm] |           | [mm]           | [mm] | [kg (lb)]      |                      |
| 25                         | 10 | 125  | 14   | 67   | 1    | 4         | 19             | 90   | 1.5 (3.31)     | KC                   |
| 50                         | 10 | 155  | 16   | 96   | 2    | 4         | 19             | 120  | 2.3 (5.07)     | KF                   |
| 80                         | 10 | 185  | 18   | 127  | 2    | 8         | 19             | 150  | 3.3 (7.28)     | KL                   |
| 100                        | 10 | 210  | 18   | 151  | 2    | 8         | 19             | 175  | 4.4 (9.7)      | KH                   |


- 1) Material: AISI 316L
- 2) The roughness of the surface in contact with the medium, including the raised face of the flanges (all standards) made of Alloy C276, Monel, tantalum, gold or PTFE, is  $R_a < 0.8 \mu\text{m}$  ( $31.5 \mu\text{in}$ ). Lower surface roughness available on request.
- 3) The flange raised face is made of the same material as the process membrane.
- 4) Product Configurator, order code for "Process connection"

Maximum diameter of the process membrane  $\varnothing d_M$

| A <sup>1)</sup> | K <sup>2)</sup> | $\varnothing d_M$ (mm) |      |            |          |                   |      |
|-----------------|-----------------|------------------------|------|------------|----------|-------------------|------|
|                 |                 | 316L TempC             | 316L | Alloy C276 | Tantalum | Monel (Alloy 400) | PTFE |
| 25              | 10              | -                      | 28   | -          | -        | -                 | -    |
| 40              | 10              | -                      | 38   | -          | -        | -                 | -    |
| 50              | 10              | -                      | 52   | 62         | 60       | 59                | -    |
| 80              | 10              | -                      | 80   | -          | -        | -                 | -    |
| 100             | 10              | -                      | 80   | -          | -        | -                 | -    |

- 1) Alphanumeric designation of the flange size.
- 2) Alphanumeric pressure rating of a component.


Process connections PMP75 Welded separators

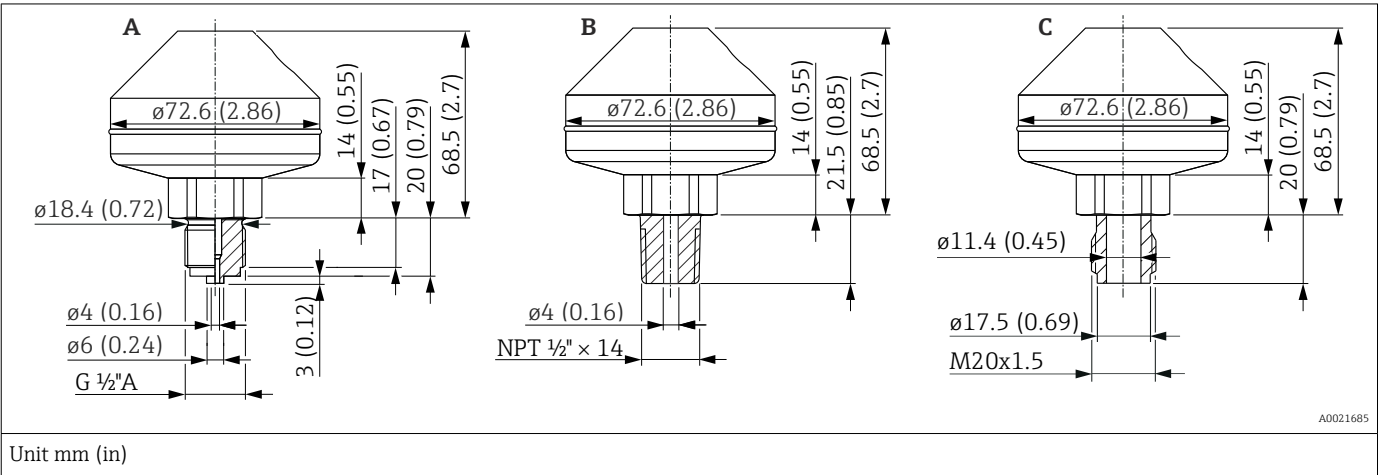

| Item | Designation                    | Material  | Measuring range | PN  | Weight      | Option <sup>1)</sup> |
|------|--------------------------------|-----------|-----------------|-----|-------------|----------------------|
|      |                                |           | [bar (psi)]     |     | [kg (lb)]   |                      |
| A    | Welded, ISO 228 G 1/2 A EN 837 | AISI 316L | ≤ 160 (2320)    | 160 | 1.43 (3.15) | UA                   |
| B    | Welded, ANSI 1/2 MNPT          |           |                 |     |             | UB                   |
| C    | Welded, DIN 13 M20x1.5 thread  |           |                 |     |             | UF                   |

1) Product Configurator, order code for "Process connection"


Threaded separators, PN100, TempC

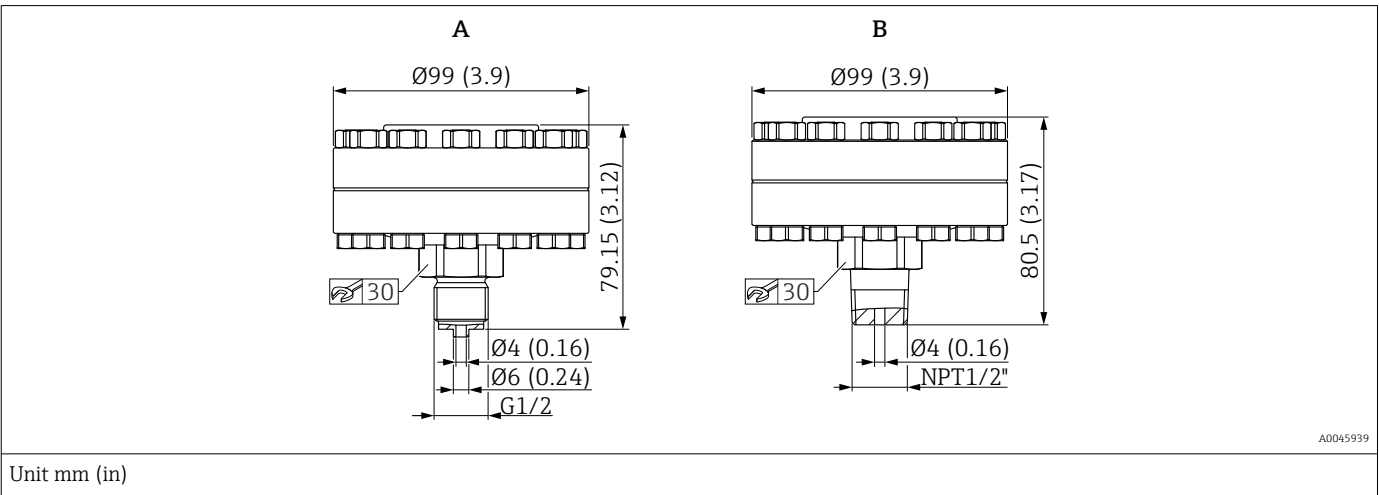

| Item | Designation                                                                                     | Material                        | Measuring range | PN | Weight            | Option <sup>1)</sup> |
|------|-------------------------------------------------------------------------------------------------|---------------------------------|-----------------|----|-------------------|----------------------|
|      |                                                                                                 |                                 | bar (psi)       |    | kg (lb)           |                      |
| A    | Threaded, ISO228 G 1/2 EN837 with metal seal (silver-plated)<br>-60 to +400 °C (-76 to +752 °F) | AISI 316L,<br>screws made of A4 | ≤ 40 (580)      | 40 | 2.35 kg (5.18 lb) | UC                   |
| B    | Threaded, ASME MNPT 1/2 with metal seal (silver-plated)<br>-60 to +400 °C (-76 to +752 °F)      |                                 |                 |    | 2.35 kg (5.18 lb) | UD                   |

1) Product Configurator, order code for "Process connection"


## Threaded separators, PN250

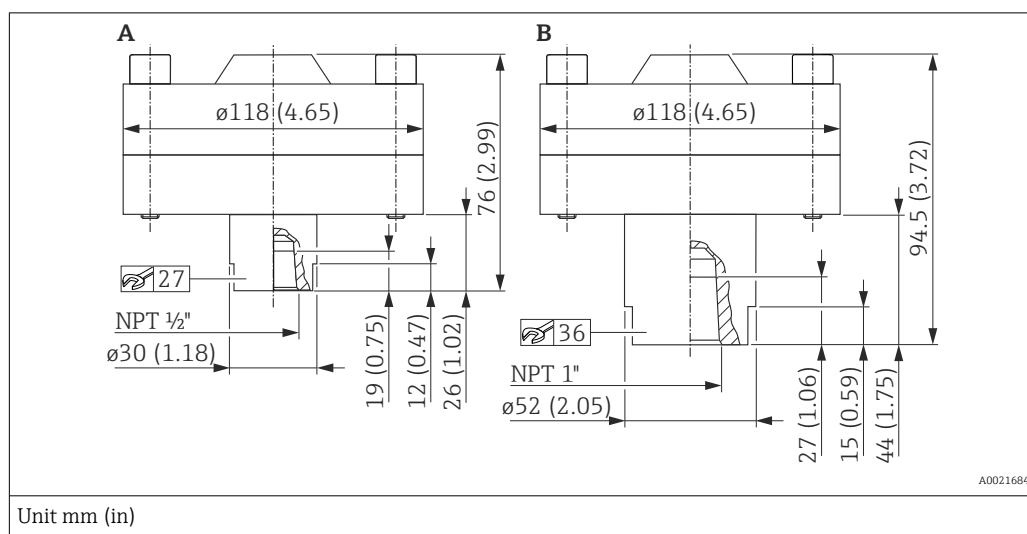

| Item | Designation                                                     | Material                       | Measuring range | PN  | Weight       | Option <sup>1)</sup> |
|------|-----------------------------------------------------------------|--------------------------------|-----------------|-----|--------------|----------------------|
|      |                                                                 |                                | [bar (psi)]     |     | [kg (lb)]    |                      |
| A    | Threaded, 1/2" NPT with FKM seal -20 to +200 °C (-4 to +392 °F) | AISI 316L<br>Screws made of A4 | ≤ 250 (3625)    | 250 | 4.75 (10.47) | UG                   |
| B    | Threaded, 1" NPT with FKM seal -20 to +200 °C (-4 to +392 °F)   |                                |                 |     | 5.0 (11.03)  | UH                   |

1) Product Configurator, order code for "Process connection"


Threaded separators, PN400

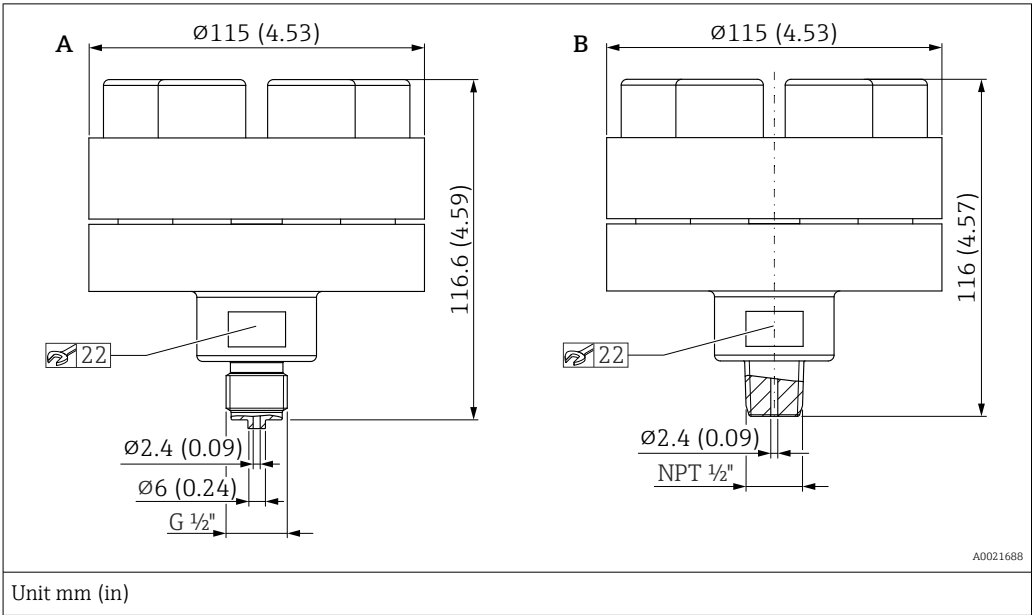

| Item | Designation                                                                                | Material                        | Measuring range | PN <sup>1)</sup> | Weight       | Option <sup>2)</sup> |
|------|--------------------------------------------------------------------------------------------|---------------------------------|-----------------|------------------|--------------|----------------------|
|      |                                                                                            |                                 | [bar (psi)]     |                  | [kg (lb)]    |                      |
| A    | Threaded, ISO 228 G ½ A EN837, with integrated seal lip<br>-60 to +400 °C (-76 to +752 °F) | AISI 316L,<br>screws made of A4 | > 40 (580)      | 400              | 4.75 (10.47) | UC                   |
| B    | Threaded, ANSI ½ MNPT, with integrated seal lip<br>-60 to +400 °C (-76 to +752 °F)         |                                 |                 |                  |              | UD                   |

- 1) This separator is assembled prior to delivery and must not be disassembled!
- 2) Product Configurator, order code for "Process connection"


# Separate housing: Wall and pipe mounting with mounting bracket

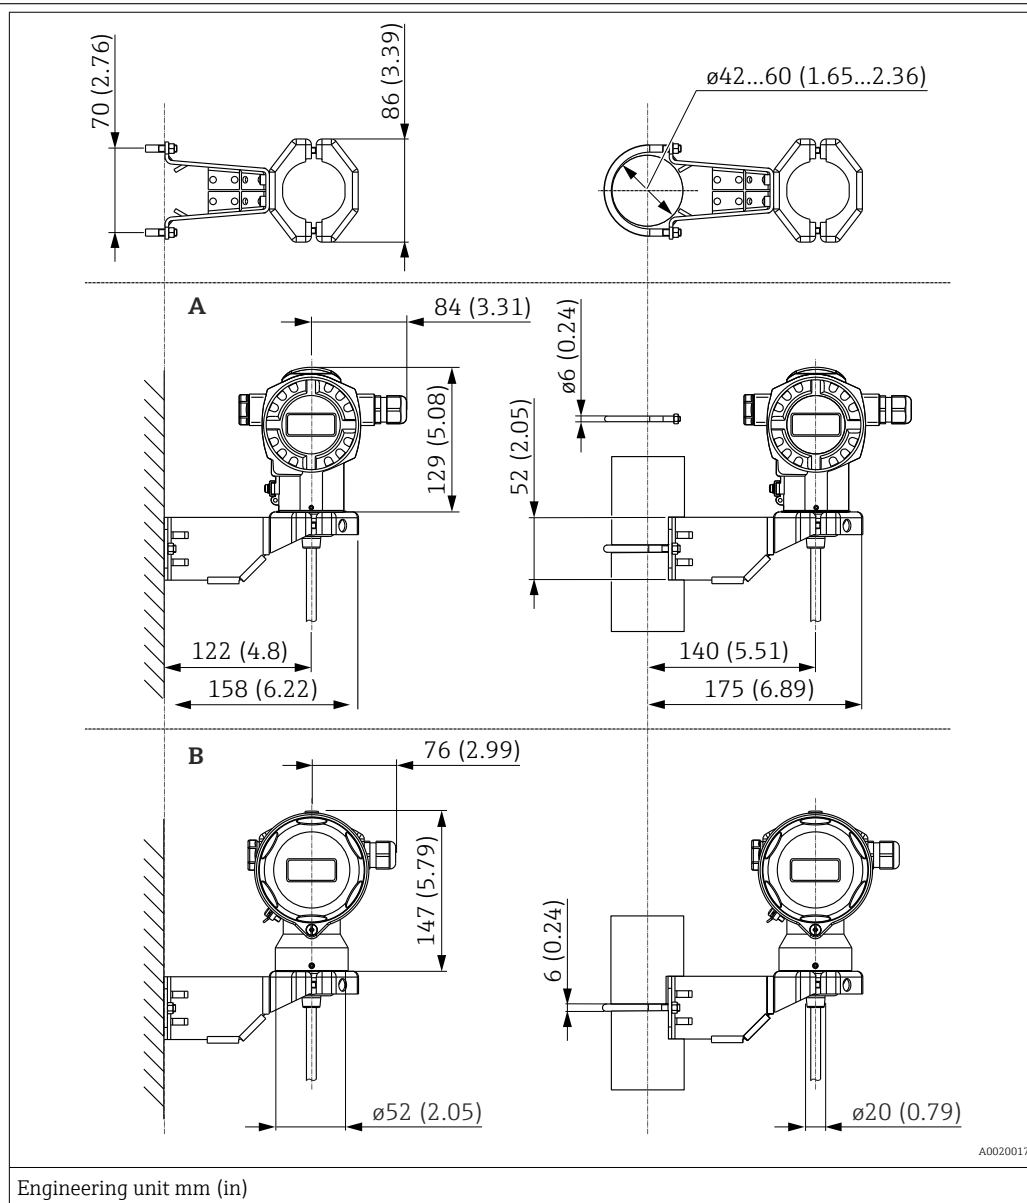

| Item | Designation                                        | Weight in kg (lb)    |                  | Option <sup>1)</sup> |
|------|----------------------------------------------------|----------------------|------------------|----------------------|
|      |                                                    | Housing (T14 or T17) | Mounting bracket |                      |
| A    | Dimensions with T14 housing, optional side display | → 51                 | 0.5 (1.10)       | U                    |
| B    | Dimensions with T17 housing, optional side display |                      |                  |                      |

1) Product Configurator, order code for "Additional options 2", version "G"

Also available for order as a separate accessory: part number 71102216

**Flushing rings**

A0028007

Use flushing rings if there is a risk of medium buildup or clogging at the process connection. The flushing ring is fitted between the process connection and the process connection provided by the customer.

Using the two lateral flushing holes, medium buildup or clogging in front of the process membrane can be rinsed away and the pressure chamber vented.

Various nominal widths and forms allow adaption to the respective process flange.

For other details (dimension, weight, materials), see SD01553P/00/EN "Mechanical accessories for pressure measuring instruments".

**Order options**

Flushing rings can be ordered as a separate accessory or as an order option for the device.

| Material  | Nominal diameter | Accessory <sup>1)</sup><br>Part number | Order option <sup>2) 3)</sup> |
|-----------|------------------|----------------------------------------|-------------------------------|
|           |                  |                                        | PMP75                         |
| AISI 316L | EN1092-1         |                                        |                               |
|           | DN25             | 71377379                               | PO                            |
|           | DN50             | 71377380                               | PP                            |
|           | DN80             | 71377383                               | PQ                            |
|           | ASME B16.5       |                                        |                               |
|           | NPS 1"           | 71377369                               | PK                            |
|           | NPS 2"           | 71377370                               | PL                            |
|           | NPS 3"           | 71377371                               | PM                            |

1) Inspection certification according to EN10204-3.1 material

2) Product Configurator, order code for "Accessories enclosed"

3) Certificates ordered with the equipment (3.1 Material certificate and NACE Declaration of Conformity and PMI tests) apply to the transmitters and flushing rings listed in the table.


Endress+Hauser offers additional flushing rings as **Technical Special Products (TSP)**.

**Weight**

| Component                                          | Weight                                    |
|----------------------------------------------------|-------------------------------------------|
| Housing                                            | See "Housing" section                     |
| Process connection                                 | See "Process connections" section         |
| Temperature isolator                               | 0.34 kg (0.75 lb)                         |
| Capillary with armoring made of AISI 316L (1.4404) | 0.16 kg/m (0.35 lb/m) + 0.35 kg (0.77 lb) |
| Capillary with armoring made of AISI 316L (PVC)    | 0.21 kg/m (0.46 lb/m) + 0.35 kg (0.77 lb) |
| Capillary with armoring made of AISI 316L (PTFE)   | 0.29 kg/m (0.64 lb/m) + 0.35 kg (0.77 lb) |


# Materials not in contact with process

## Transmitter housing

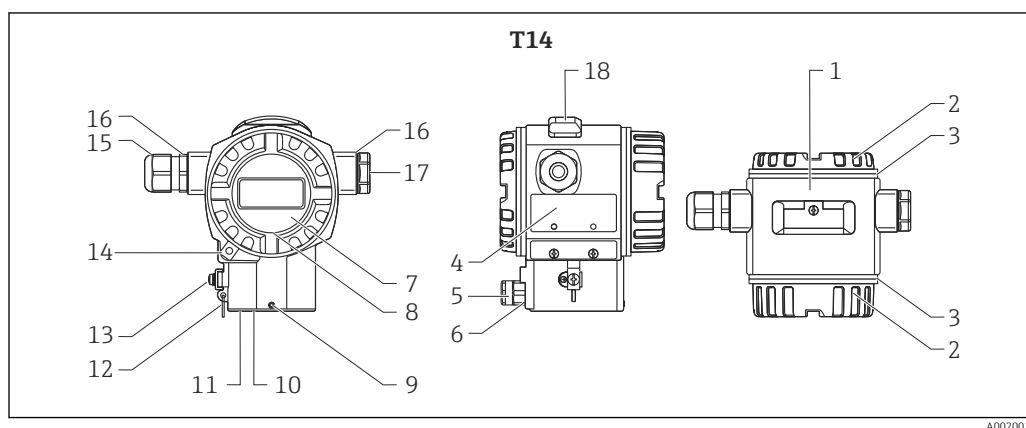

A0020019


| Item number                        | Component                                                | Material                                                                                                                                                                       |
|------------------------------------|----------------------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1                                  | T14 housing, RAL 5012 (blue)                             | <ul style="list-style-type: none"> <li>Die-cast aluminum with protective powder-coating on polyester base</li> <li>Coating on thread: Heat-curing lubricant varnish</li> </ul> |
| 1                                  | T14 housing                                              | <ul style="list-style-type: none"> <li>Precision casting AISI 316L (1.4435)</li> <li>Coating on thread: Heat-curing lubricant varnish</li> </ul>                               |
| 2                                  | Cover, RAL 7035 (gray)                                   | Die-cast aluminum with protective powder-coating on polyester base<br>Precision cast AISI 316L (1.4435) (cover made of 316L if T14 housing made of 316L)                       |
| 4                                  | Nameplates                                               | <ul style="list-style-type: none"> <li>AISI 316L (1.4404), if T14 housing is precision-cast</li> <li>Anodized aluminum, if housing T14/T15 of die-cast aluminum</li> </ul>     |
| 5                                  | Pressure compensation filter                             | AISI 316L (1.4404) and PBT-FR                                                                                                                                                  |
| 6                                  | Pressure compensation filter, O-ring                     | VMQ or EPDM                                                                                                                                                                    |
| 7                                  | Sight glass                                              | Mineral glass                                                                                                                                                                  |
| 8                                  | Sight glass seal                                         | Silicone (VMQ)                                                                                                                                                                 |
| 9                                  | Screw                                                    | A4                                                                                                                                                                             |
| 10                                 | Sealing ring                                             | EPDM                                                                                                                                                                           |
| 11                                 | Snap ring                                                | PA66-GF25                                                                                                                                                                      |
| 12                                 | Rope for nameplates                                      | AISI 316 (1.4401)                                                                                                                                                              |
| 13                                 | External ground terminal                                 | AISI 316L (1.4404)                                                                                                                                                             |
| 14                                 | Cover clamp                                              | AISI 316L (1.4435) clamp, A4 screw                                                                                                                                             |
| 15                                 | Cable entry                                              | Polyamide (PA) or CuZn nickel-plated                                                                                                                                           |
| 16                                 | Seal of cable entry and plug                             | Silicone (VMQ)                                                                                                                                                                 |
| 17                                 | Plug                                                     | PBT-GF30 FR, for dust ignition-proof and Exd: AISI 316L (1.4435)                                                                                                               |
| 18                                 | External operation (keys and key cover), RAL 7035 (gray) | Polycarbonate PC-FR, screw A4                                                                                                                                                  |
| Devices with MID parts certificate | Seal wire                                                | DIN 1367-0 St/Zn (soft galvanized steel)                                                                                                                                       |
| Devices with MID parts certificate | Seals                                                    | Pb (lead)                                                                                                                                                                      |

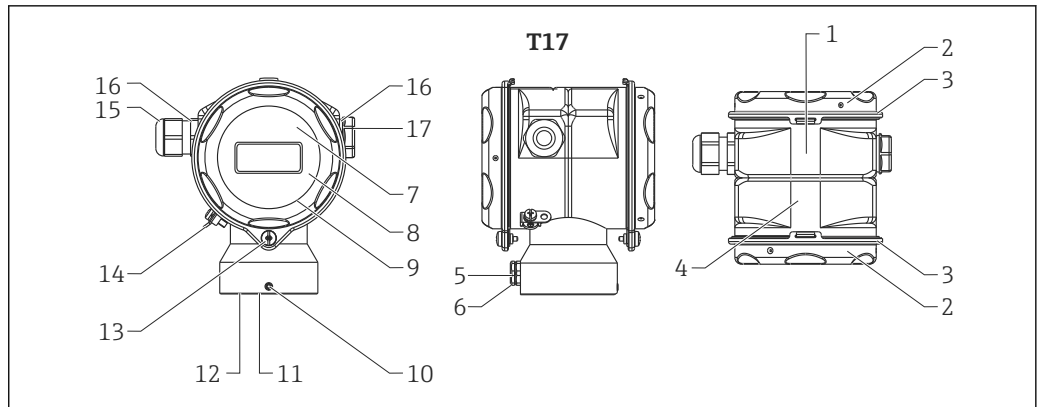

A0020021


| Item number                        | Component                                                                                                        | Material                                                  |
|------------------------------------|------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------|
| 1                                  | T17 housing                                                                                                      | AISI 316L (1.4404)                                        |
| 2                                  | Cover                                                                                                            |                                                           |
| 3                                  | Cover seal                                                                                                       |                                                           |
| 4                                  | Nameplates                                                                                                       | Lasered on                                                |
| 5                                  | Pressure compensation filter                                                                                     | AISI 316L (1.4404) and PBT-FR                             |
| 6                                  | Pressure compensation filter, O-ring                                                                             | VMQ or EPDM                                               |
| 7                                  | Sight glass for non-hazardous area, ATEX Ex ia, NEPSI Zone 0/1 Ex ia, IECEx Zone 0/1 Ex ia, FM NI, FM IS, CSA IS | Polycarbonate (PC)                                        |
| 8                                  | Sight glass for ATEX 1/2 D, ATEX 1/3 D, ATEX 1 GD, ATEX 1/2 GD, ATEX 3 G, FM DIP, CSA dust ignition-proof        | Mineral glass                                             |
| 9                                  | Sight glass seal                                                                                                 | EPDM                                                      |
| 10                                 | Screw                                                                                                            | A2-70                                                     |
| 11                                 | Sealing ring                                                                                                     | EPDM                                                      |
| 12                                 | Snap ring                                                                                                        | PA6                                                       |
| 13                                 | Screw                                                                                                            | A4-50<br>Coating on thread: Heat-curing lubricant varnish |
| 14                                 | External ground terminal                                                                                         | AISI 316L (1.4404)                                        |
| 15                                 | Cable entry                                                                                                      | Polyamide PA, for dust ignition-proof: CuZn nickel-plated |
| 16                                 | Seal of cable entry and plug                                                                                     | Silicone (VMQ)                                            |
| 17                                 | Plug                                                                                                             | PBT-GF30 FR, for dust ignition-proof: AISI 316L (1.4435)  |
| Devices with MID parts certificate | Seal wire                                                                                                        | DIN 1367-0 St/Zn (soft galvanized steel)                  |
| Devices with MID parts certificate | Seals                                                                                                            | Pb (lead)                                                 |

## Connecting parts

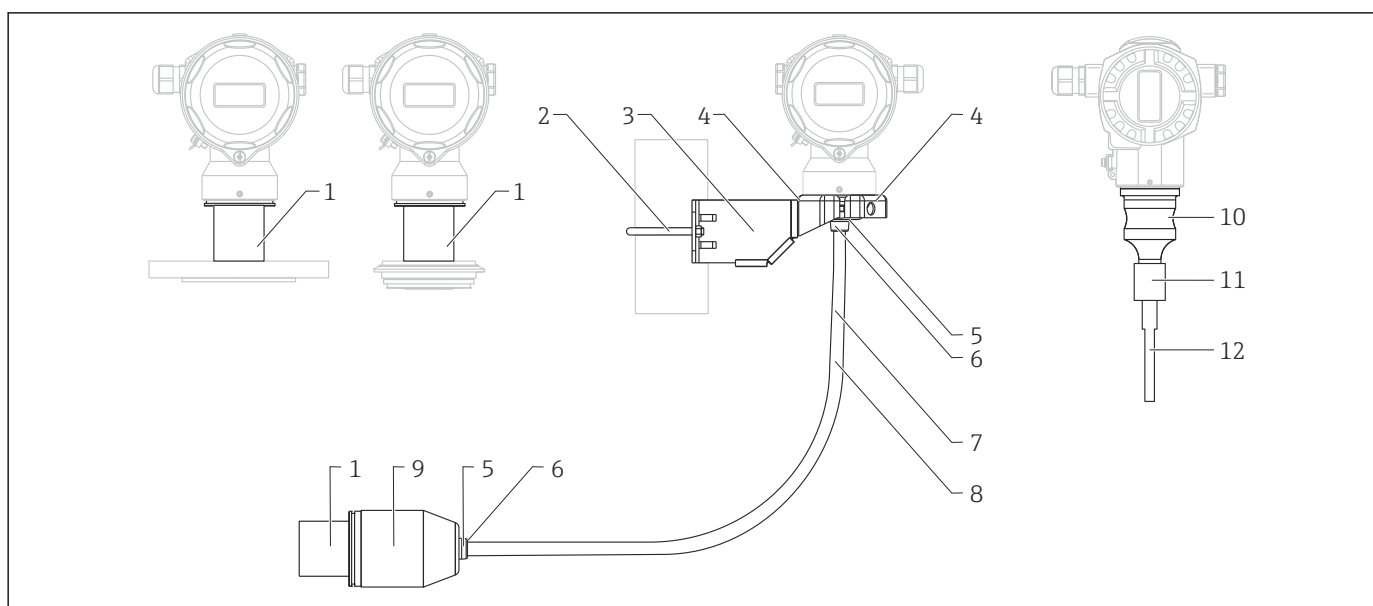

A0028222

| Item number | Component                                                                | Material                                                                                                                                                                        |
|-------------|--------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| 1           | Connection between the housing and process connection                    | AISI 316L (1.4404)                                                                                                                                                              |
| 2           | Mounting bracket                                                         | Bracket AISI 316L (1.4404)                                                                                                                                                      |
| 3           |                                                                          | Screw and nuts A4-70                                                                                                                                                            |
| 4           |                                                                          | Half-shells: AISI 316L (1.4404)                                                                                                                                                 |
| 5           | Seal for cable of separate housing                                       | EPDM                                                                                                                                                                            |
| 6           | Gland for cable from separate housing                                    | AISI 316L (1.4404)                                                                                                                                                              |
| 7           | PE cable for separate housing                                            | Abrasion-resistant cable with Dynema strain-relief members; shielded with aluminum-coated film; insulated with polyethylene (PE-LD), black; copper wires, twisted, UV-resistant |
| 8           | FEP cable for separate housing                                           | Abrasion-resistant cable; shielded with galvanized steel wire netting; insulated with fluorinated ethylene propylene (FEP), black; copper wires, twisted, UV-resistant          |
| 9           | Process connection adapter for separate housing                          | AISI 316L (1.4404)                                                                                                                                                              |
| 10          | Cell body                                                                | AISI 316L (1.4404)                                                                                                                                                              |
| 11          | Connection between body of measuring cell and capillary                  | AISI 316L (1.4404)                                                                                                                                                              |
| 12          | Heat-shrink tube<br>(available only if capillary has PTFE or PVC sheath) | Polyolefin                                                                                                                                                                      |

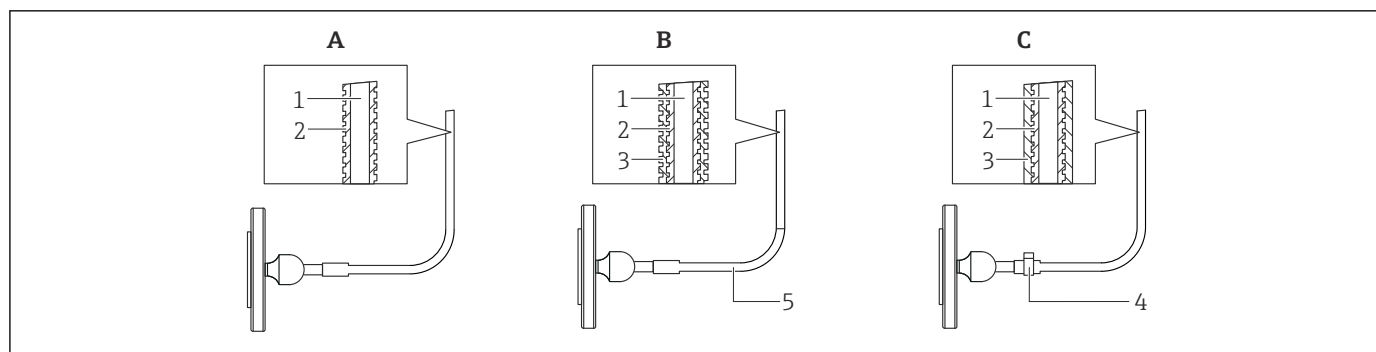

A0028087

| Item | Component                           | A<br>Standard <sup>1)</sup><br>Armor for capillary | B<br>PVC-coated<br>Armor for capillary | C<br>PTFE hose<br>Armor for capillary |
|------|-------------------------------------|----------------------------------------------------|----------------------------------------|---------------------------------------|
| 1    | Capillary                           | AISI 316 Ti (1.4571)                               | AISI 316 Ti (1.4571)                   | AISI 316 Ti (1.4571)                  |
| 2    | Flexible armor for capillary        | AISI 316L (1.4404) <sup>2)</sup>                   | AISI 316L (1.4404)                     | AISI 316L (1.4404)                    |
| 3    | Coating/armor                       | -                                                  | PVC <sup>3)</sup>                      | PTFE <sup>4)</sup>                    |
| 4    | Single-ear clamp                    | -                                                  | -                                      | 1.4301                                |
| 5    | Shrink tubing at capillary junction | -                                                  | Polyolefin                             | -                                     |

- 1) If no option is specified when ordering, order option "SA" is supplied.  
 2) Product Configurator, order code for "Armor for capillary:" option "SA"  
 3) Product Configurator, order code for "Armor for capillary:" option "SB"  
 4) Product Configurator, order code for "Armor for capillary:" option "SC"

#### Materials in contact with process

##### NOTICE

- ▶ Device components in contact with the process are listed in the "Mechanical construction" → 50 and "Ordering information" → 124 sections.

#### Delta ferrite content

A delta ferrite content of  $\leq 3\%$  can be guaranteed and certified for the wetted parts if option "8" is selected in the "Additional options 1" or "Additional options 2" order code in the Product Configurator.

If the PMC71 with hygienic process connections is selected, a delta ferrite content of  $\leq 1\%$  can be guaranteed and certified if option "8" is selected in the "Additional options 1" or "Additional options 2" order code in the Product Configurator.

#### TSE Certificate of Suitability (Transmissible Spongiform Encephalopathy)

The following applies to all device components in contact with the process:

- They do not contain any materials derived from animals.
- No additives or operating materials derived from animals are used in production or processing.

#### Process connections

- "Clamp connections" and "Hygienic process connections": AISI 316L (DIN/EN material number 1.4435)
- Endress+Hauser supplies threaded process connections and DIN/EN flanges in stainless steel according to AISI 316L (DIN/EN material number 1.4404 or 1.4435). With regard to their stability-temperature property, the materials 1.4404 and 1.4435 are grouped together under 13EO in EN 1092-1: 2001 Tab. 18. The chemical composition of the two materials can be identical.
- Some process connections are also available in Alloy C276 (DIN/EN material number 2.4819). For this purpose see the information in the "Mechanical construction" section.

**Process membrane**

| Measuring cell | Designation                                                                                                                                                                                  | Option <sup>1)</sup> |
|----------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------------|
| PMC71          | Al <sub>2</sub> O <sub>3</sub> aluminum oxide ceramic FDA, ultrapure 99.9 % <sup>2)</sup><br>Ceraphire® (see also <a href="http://www.endress.com/ceraphire">www.endress.com/ceraphire</a> ) | Standard             |
| PMP71          | AISI 316L                                                                                                                                                                                    | 1                    |
|                | AISI 316L with gold-rhodium coating                                                                                                                                                          | 6                    |
|                | Alloy C276 (2.4819)                                                                                                                                                                          | 2                    |
| PMP75          | AISI 316L with gold coating (25 µm), TempC <sup>3)</sup>                                                                                                                                     | G                    |
|                | AISI 316L                                                                                                                                                                                    | 1                    |
|                | AISI 316L, TempC <sup>3)</sup>                                                                                                                                                               | E                    |
|                | AISI 316L with gold-rhodium coating                                                                                                                                                          | 6                    |
|                | AISI 316L with 0.25 mm (0.01 in) PTFE coating                                                                                                                                                | 8                    |
|                | Alloy C276 (2.4819)                                                                                                                                                                          | 2 <sup>4)</sup>      |
|                | Monel (2.4360)                                                                                                                                                                               | 3 <sup>4)</sup>      |
|                | AISI 316L with gold coating                                                                                                                                                                  | 4                    |
|                | Tantalum (UNS R05200)                                                                                                                                                                        | 5 <sup>4)</sup>      |

- 1) Product Configurator, order code for "Membrane material"
- 2) The US Food & Drug Administration (FDA) has no objections to the use of ceramics made from aluminum oxide as a surface material in contact with foodstuffs. This declaration is based on the FDA certificates of our ceramic suppliers
- 3) The TempC gold-plated membrane does not offer corrosion protection!
- 4) The material of the flange raised face is the same as that used for the process membrane. For devices with a barrel (extended diaphragm seal), the raised face of the flange and the barrel pipe are made from 316L.

**Seals**

| Device | Designation                                                                       | Option <sup>1)</sup> |
|--------|-----------------------------------------------------------------------------------|----------------------|
| PMC71  | FKM                                                                               | A                    |
|        | FKM, FDA                                                                          | G                    |
|        | EPDM                                                                              | B                    |
|        | FFKM Perlast G75LT                                                                | C                    |
|        | Kalrez                                                                            | D                    |
|        | Chemraz                                                                           | E                    |
|        | NBR (FDA)/3A: HNBR (FDA)                                                          | F                    |
|        | FKM, cleaned for PWIS-free applications                                           | L                    |
|        | Kalrez, cleaned for PWIS-free applications                                        | M                    |
|        | FKM, cleaned of oil+grease                                                        | 1                    |
|        | FKM, cleaned for oxygen service, note pressure and temperature application limits | 2                    |

- 1) Product Configurator, order code for "Seal"

**Fill fluid**
**PMP71**

| Designation                                                                             | Option <sup>1)</sup> |
|-----------------------------------------------------------------------------------------|----------------------|
| Silicone oil                                                                            | A                    |
| Inert oil                                                                               | F                    |
| Inert oil, cleaned from oil and grease                                                  | K                    |
| Inert oil, cleaned for oxygen service (observe application limits pressure/temperature) | N                    |

1) Product Configurator, order code for "Fill fluid"

**PMP75**

| Designation                                                       | Option <sup>1) 2)</sup> |
|-------------------------------------------------------------------|-------------------------|
| Silicone oil (food-safe FDA 21 CFR 175.105)                       | A                       |
| ...m capillary, inert oil                                         | B                       |
| ...ft capillary, inert oil                                        | C                       |
| Vegetable oil (food-safe FDA 21 CFR 172.856)                      | D                       |
| Inert oil                                                         | F                       |
| High-temperature oil, temperature isolator                        | G                       |
| Silicone oil, temperature isolator (food-safe FDA 21 CFR 175.105) | H                       |
| Vegetable oil, temperature isolator                               | J                       |
| Inert oil, cleaned from oil and grease                            | K                       |
| Inert oil, cleaned for oxygen service                             | N                       |
| ...m capillary, silicone oil (food-safe FDA 21 CFR 175.105)       | 1                       |
| ...ft capillary, silicone oil (food-safe FDA 21 CFR 175.105)      | 2                       |
| ...m capillary, high-temperature oil                              | 3                       |
| ...ft capillary, high-temperature oil                             | 4                       |
| ...m capillary, vegetable oil (food-safe FDA 21 CFR 172.856)      | 5                       |
| ...ft capillary, vegetable oil (food-safe FDA 21 CFR 172.856)     | 6                       |
| ...m capillary, low-temperature oil                               | 7                       |
| ...ft capillary, low-temperature oil                              | 8                       |

1) Product Configurator, order code for "Fill fluid"

2) For diaphragm seal devices with 3-A and EHEDG certificates, only select fill fluid with FDA approval

## Operability

### Operating concept

#### Operator-oriented menu structure for user-specific tasks

- Commissioning
- Operation
- Diagnosis

#### Quick and safe commissioning

Guided menus for applications

#### Reliable operation

- Local operation possible in several languages
- Standardized operation at the device and in the operating tools
- Parameters relating to measured values can be locked/unlocked using the device's write protection switch, using the device software or via remote operation

#### Efficient diagnostics increase measurement availability

- Remedial measures are integrated in plain text
- Diverse simulation options

### Local operation

#### Functions

| Function                                                                                   | External operation<br>(operating keys,<br>optional, not T17<br>housing) | Internal operation<br>(electronic insert) | Onsite display<br>(optional) |
|--------------------------------------------------------------------------------------------|-------------------------------------------------------------------------|-------------------------------------------|------------------------------|
| Position adjustment (zero point correction)                                                | ✓                                                                       | ✓                                         | ✓                            |
| Setting lower range value and upper range value - reference pressure present at the device | ✓<br>(HART only)                                                        | ✓<br>(HART only)                          | ✓                            |
| Device reset                                                                               | ✓                                                                       | ✓                                         | ✓                            |
| Locking and unlocking parameters relevant to the measured value                            | —                                                                       | ✓                                         | ✓                            |
| Value acceptance indicated by the green LED                                                | ✓                                                                       | ✓                                         | ✓                            |
| Switching damping on and off                                                               | ✓<br>(only if display is<br>connected)                                  | ✓<br>(HART and PA only)                   | ✓                            |
| Configuring the bus address of the device (PA)                                             | —                                                                       | ✓                                         | ✓                            |
| Switching simulation mode on and off (FOUNDATION Fieldbus)                                 | —                                                                       | ✓                                         | ✓                            |

#### Operating the device using onsite display (optional)

A 4-line liquid crystal display (LCD) is used for display and operation. The onsite display shows measured values, dialog text as well as fault and notice messages in plain text, thereby supporting the user in every stage of operation.

The display can be removed for easy operation.


The device display can be turned in 90° steps.

Depending on the installation position of the device, this makes it easy to operate the device and read the measured value.

#### Functions:

- 8-digit measured value display including sign and decimal point and bar graph for
  - 4 to 20 mA HART (bar graph from 4 to 20 mA)
  - 1-5V DC (bar graph from 1 to 5 volt)
  - PROFIBUS PA (bar graph as graphic display of standardized value of AI block)
  - FOUNDATION Fieldbus (bar graph as graphic display of transducer output).
- Simple and complete menu guidance due to breakdown of parameters into several levels and groups.
- Menu guidance in up to 8 languages
- Each parameter is given a 3-digit ID number for easy navigation.
- Option for configuring the display according to individual requirements and preferences, such as language, alternating display, display of other measured values such as sensor temperature, contrast setting.
- Comprehensive diagnostic functions (fault and warning message, peak-hold indicators, etc.).
- Rapid and safe commissioning with the Quick Setup menus

#### Overview

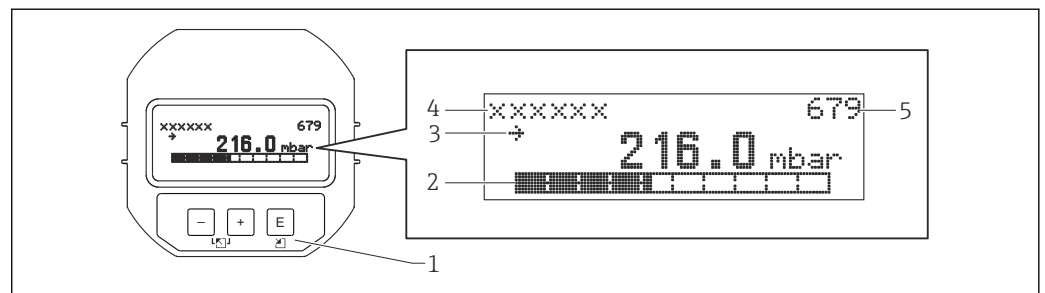


A0016498

- 1 Operating keys
- 2 Bargraph
- 3 Symbol
- 4 Header
- 5 Parameter ID number

#### Operating keys on the exterior of the device

With the aluminum housing (T14), the operating keys are located either outside on the housing, under the protection cap or inside on the electronic insert. With the stainless steel housing (T17), the operating keys are always located inside the housing on the electronic insert.

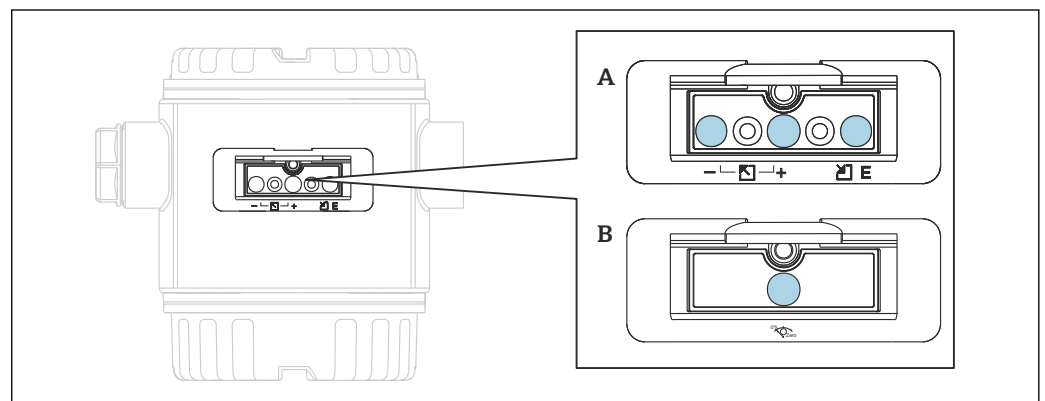

A0020030

- A 1-5V DC and 4 to 20 mA HART
- B PROFIBUS PA and FOUNDATION Fieldbus

The operating keys located externally on the device work on the Hall sensor principle. As a result, no additional openings are required in the device. This guarantees:

- Complete protection against environmental influences such as moisture and contamination.
- Simple operation without any tools.
- No wear.

Ordering information:


Product Configurator, order code for "Output, operation"

### Operating keys and elements located internally on the electronic insert

Ordering information:

Product Configurator, order code for "Output, operation"


#### HART

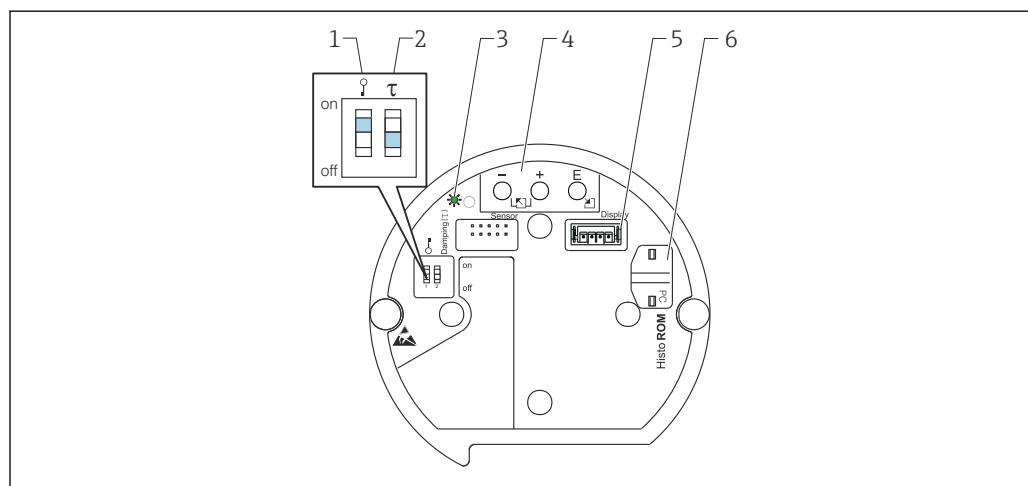

A0020031

- 1 DIP switch for locking/unlocking parameters relevant to the measured value
- 2 DIP switch for switching damping on/off
- 3 Green LED to indicate value being accepted
- 4 Operating keys
- 5 Slot for optional display
- 6 Slot for optional HistoROM®/M-DAT


#### 1-5V DC

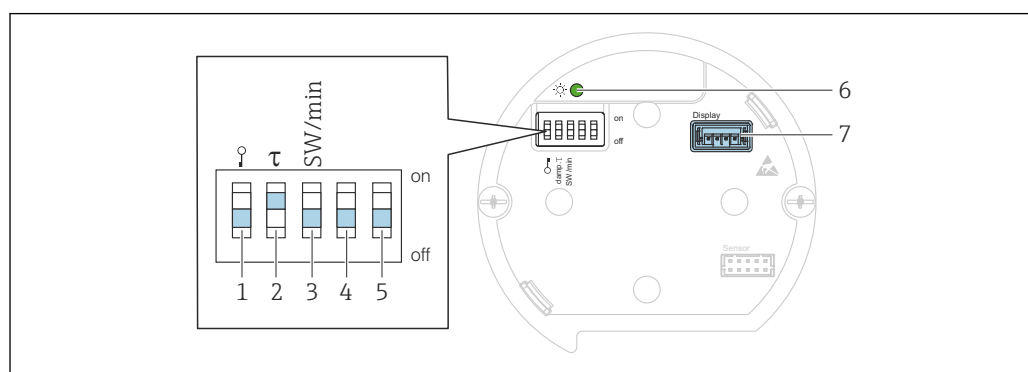

A0031800

- 1 DIP switch for locking/unlocking parameters relevant to the measured value
- 2 DIP switch for switching damping on/off
- 3 DIP switch for alarm voltage/alarm current SW / alarm min (0.9 V/~3.6 mA)
- 4...5 Not assigned
- 6 Green LED to indicate value being accepted
- 7 Slot for display


PROFIBUS PA

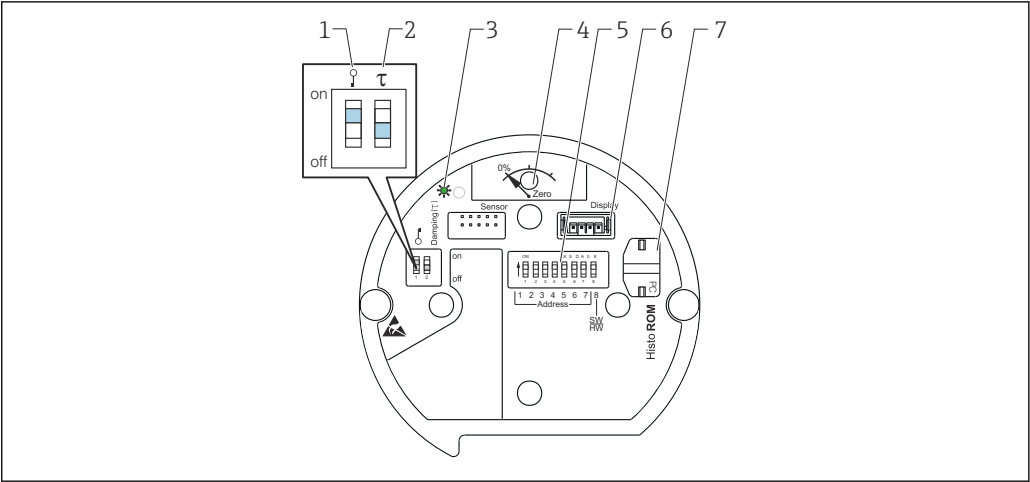

A0020032

- 1 DIP switch for locking/unlocking parameters relevant to the measured value
- 2 DIP switch for switching damping on/off
- 3 Green LED to indicate value being accepted
- 4 Key for position adjustment and device reset
- 5 DIP switch for bus address
- 6 Slot for optional display
- 7 Slot for optional HistoROM®/M-DAT

FOUNDATION Fieldbus

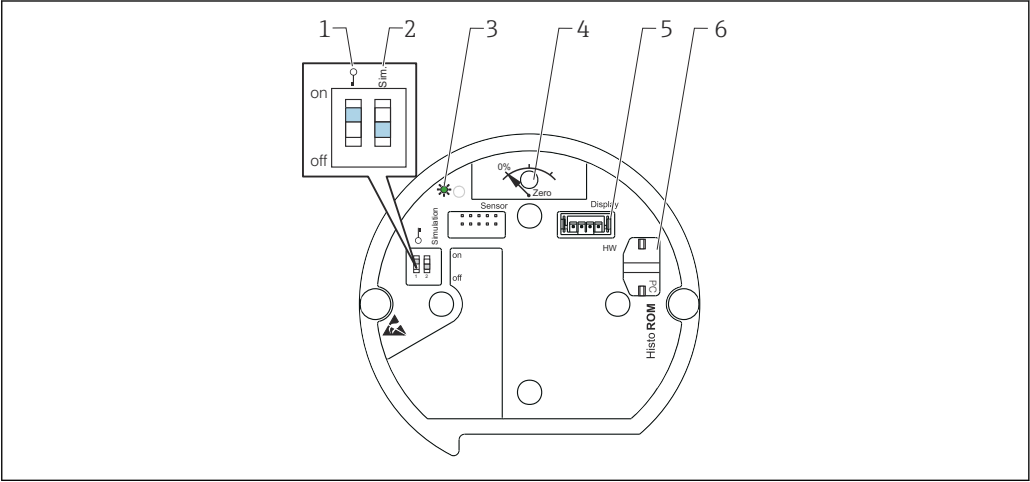

A0020033

- 1 DIP switch for locking/unlocking parameters relevant to the measured value
- 2 DIP switch for simulation mode on/off
- 3 Green LED to indicate value being accepted
- 4 Key for position adjustment and device reset
- 5 Slot for optional display
- 6 Slot for optional HistoROM®/M-DAT

Remote operation

All software parameters are accessible depending on the position of the write protection switch on the device.

| Hardware and software for remote operation <sup>1)</sup> | HART | PROFIBUS PA | FOUNDATION Fieldbus |
|----------------------------------------------------------|------|-------------|---------------------|
| FieldCare                                                | ✓    | ✓           | ✓                   |
| FieldXpert SFX100                                        | ✓    | —           | ✓                   |

| Hardware and software for remote operation<br>1) | HART | PROFIBUS PA | FOUNDATION Fieldbus |
|--------------------------------------------------|------|-------------|---------------------|
| NI-FBUS Configurator                             | —    | —           | ✓                   |
| HistoROM®/M-DAT                                  | ✓    | ✓           | ✓                   |

1) Not for 1-5V DC

### FieldCare

FieldCare is an Endress+Hauser asset management tool based on FDT technology. With FieldCare, you can configure all Endress+Hauser devices as well as devices from other manufacturers that support the FDT standard.

FieldCare supports the following functions:

- Configuration of transmitters in offline and online mode
- Device data upload/download (not for 1-5V DC)
- HistoROM®/M-DAT analysis
- Documentation of the measuring point

Connection options:

- HART via Commubox FXA195 and USB interface of a computer
- PROFIBUS PA via segment coupler and PROFIBUS interface card
- Service interface with Commubox FXA291 and ToF adapter FXA291 (USB).



For further information, please contact your local Endress+Hauser Sales Center.

### Field Xpert SFX100

Field Xpert is an industrial PDA with integrated 3.5" touchscreen from Endress+Hauser based on Windows Mobile. It offers wireless communication via the optional VIATOR Bluetooth modem from Endress+Hauser. Field Xpert also works as a stand-alone device for asset management applications. For details, refer to BA00060S/04/EN.

### Commubox FXA195

For intrinsically safe HART communication with FieldCare via the USB interface. For details refer to TI00404F/00/EN.

### Commubox FXA291

The Commubox FXA291 connects Endress+Hauser field devices with a CDI interface (=Endress+Hauser Common Data Interface) to the USB interface of a personal computer or a notebook. For details refer to TI00405C/07/EN.



For the following Endress+Hauser devices you need the "ToF adapter FXA291" as an additional accessory:

- Cerabar S PMC71, PMP7x
- Deltabar S PMD7x, FMD7x
- Deltapilot S FMB70

### ToF Adapter FXA291

The ToF adapter FXA291 connects the Commubox FXA291 with devices of the ToF platform, pressure equipment and Gammapiot via the USB interface of a personal computer or a notebook. For details refer to KA00271F.

### Profiboard

For connecting a PC to the PROFIBUS.

### Proficard

For connecting a laptop to the PROFIBUS.

### FF configuration program

FF configuration program, such as NI-FBUS Configurator, to

- connect devices with "FOUNDATION Fieldbus signal" into an FF-network
- set FF-specific parameters

*Operation with NI-FBUS Configurator:*

The NI-FBUS Configurator is an easy-to-use graphical environment for creating linkages, loops, and a schedule based on the fieldbus concepts.

You can use the NI-FBUS Configurator to configure a fieldbus network as follows:

- Set block and device tags
- Set device addresses
- Create and edit function block control strategies (function block applications)
- Configure vendor-defined function and transducer blocks
- Create and edit schedules
- Read and write to function block control strategies (function block applications)
- Invoke methods specified in the manufacturer-specific DD (e.g. basic device settings)
- Display DD menus (e.g. tab for calibration data)
- Download a configuration
- Verify a configuration and compare it to a saved configuration
- Monitor a downloaded configuration
- Replace devices
- Save and print a configuration

**HistoROM®/M-DAT  
(optional)**

The HistoROM®/M-DAT is a memory module that can be attached to any electronic insert (not for 1-5V DC). HistoROM®/M-DAT can be retrofitted at any stage (order number: 52027785).

Your benefits

- Quick and safe commissioning of the same measuring points by copying the configuration data of one transmitter to another transmitter.
- Reliable process monitoring thanks to cyclical recording of pressure and sensor temperature measured values
- Simple diagnosis by recording diverse events such as alarms, configuration changes, counters for measuring range undershoot and overshoot for pressure and temperature as well as user limit overshoot and undershoot for pressure and temperature etc.
- Analysis and graphic evaluation of the events and process parameters via software (contained in scope of supply).

You can copy data from one transmitter to another transmitter when operating a FOUNDATION Fieldbus device via an FF configuration program. You need the Endress+Hauser FieldCare operating program, the Commubox FXA291 service interface and the ToF adapter FXA291 to be able to access the data and events saved in the HistoROM®/M-DAT.

Ordering information:

Product Configurator, order code for "Additional options:", version "N" or

Product Configurator, order code for "Application package:", option "EN" or

as a separate accessory (part no.: 52027785).



For further information, please contact your local Endress+Hauser Sales Center.

**System integration**

The device can be given a tag name (max. 8 alphanumeric characters).

| Designation                                          | Option <sup>1)</sup> |
|------------------------------------------------------|----------------------|
| Measuring point (TAG), see additional specifications | Z1                   |
| Bus address, see additional spec.                    | Z2                   |

1) Product Configurator, order code for "Identification"

## Planning instructions for diaphragm seal systems

### NOTICE

#### Diaphragm seal systems sized/ordered incorrectly

The performance and permitted area of application of a diaphragm seal system depend on the process membrane used, the fill fluid, the connection, the design and the prevailing process and ambient conditions.

- To help you select the right diaphragm seal systems for your particular applications, Endress+Hauser provides its customers with the "Applicator Sizing Diaphragm Seal" selection tool, which is available free of charge at [www.endress.com/applicator](http://www.endress.com/applicator) or as a download.

A0034616



For further details, or for information on an optimum diaphragm seal solution, your local Endress+Hauser Sales Center is also always happy to help.

### Applications

Diaphragm seal systems should be used if the process and the device need to be separated. Diaphragm seal systems offer clear advantages in the following instances:

- In the case of extreme process temperatures
- For aggressive media
- In the case of process media that crystallize
- In the case of corrosive or highly various process media or process media with solids content
- In the case of heterogeneous and fibrous process media
- If extreme measuring point cleaning is necessary, or in the event of very damp mounting locations
- If the measuring point is exposed to severe vibrations
- For mounting locations that are difficult to access

## Design and operation mode

Diaphragm seals are separating equipment between the measuring system and the process.

A diaphragm seal system consists of:

- A diaphragm seal
- A capillary tube or temperature isolator where applicable
- Fill fluid and
- a pressure transmitter.

The process pressure acts via the process membrane of the diaphragm seal on the liquid-filled system, which transfers the process pressure onto the sensor of the pressure transmitter.

Endress+Hauser delivers all diaphragm seal systems as welded versions. The system is hermetically sealed, which ensures the highest reliability.

The diaphragm seal determines the application range of the system by:

- The diameter of the process membrane
- The process membrane stiffness and material
- The design (oil volume)

### Diameter of process membrane

The greater the diameter of the process membrane (less stiff), the smaller the temperature effect on the measurement result.

### Stiffness of process membrane

The stiffness depends on the diameter of the process membrane, the material, any existing coating, the thickness and shape of the process membrane. The process membrane thickness and the shape are determined by the design. The stiffness of a process membrane of a diaphragm seal influences the temperature application range and the measurement error caused by temperature effects.

*The Endress+Hauser TempC process membrane: maximum accuracy and process safety during pressure and differential pressure measurement with diaphragm seals*

To measure with even greater accuracy in these applications and increase process safety, Endress+Hauser has developed the TempC process membrane which is based on a completely revolutionary technology. This process membrane guarantees the utmost level of accuracy and process safety in diaphragm seal applications.

- The very low temperature effect minimizes the effect of process temperature and ambient temperature fluctuations, thereby guaranteeing accurate and reliable measurements. Measurement inaccuracies caused by temperature are reduced to a minimum.
- The TempC process membrane can be used at temperatures between  $-70\text{ °C}$  ( $-94\text{ °F}$ ) and  $+400\text{ °C}$  ( $+752\text{ °F}$ ). This guarantees maximum process safety even in the event of very long sterilization and cleaning cycles (SIP/CIP) in tanks and pipes at high temperatures.
- Smaller instrumentation dimensions are possible thanks to the TempC process membrane. With a smaller process connection, the new process membrane measures at least as accurately as a conventional membrane with a larger diameter.
- Due to the geometry of the process membrane, an overshoot occurs initially immediately following a temperature shock. This results in a transient response, the duration and deviation of which are significantly less compared to traditional membrane types. In the case of batch processes, these shorter recovery times mean a far higher level of availability of the production facilities. The effect of the overshoot on the output signal can be reduced by setting a damping in the case of TempC process membranes.

Ordering information:

See the Product Configurator for the individual process connection and the choice of process membrane.

Selection in the Applicator:

Under "Transmitter data" in the "Membrane material" field.

### Capillary

As standard, capillaries with an internal diameter of 1 mm (0.04 in) are used.

The capillary tube influences the thermal change, the ambient temperature operating range and the response time of a diaphragm seal system as a result of its length and internal diameter.

**Fill fluid**

When selecting the fill fluid, the medium temperature and ambient temperature, as well as the process pressure, are of crucial importance. Observe the temperatures and pressures during commissioning and cleaning. A further selection criterion is the compatibility of the fill fluid with the requirements of the medium. For example, only fill fluids that do not present a health hazard may be used in the food industry, e.g. vegetable oil or silicone oil (see also the following section "Diaphragm seal fill fluids").

The fill fluid used affects the thermal change, the temperature application range of a diaphragm seal system and the response time. A change in the temperature causes a volume change of the fill fluid. The volume change is dependent on the expansion coefficient and on the volume of the fill fluid at calibration temperature (constant in the range: +21 to +33 °C (+70 to +91 °F)). The application range can be extended by a fill fluid with a lower expansion coefficient and a shorter capillary.

For example, the fill fluid expands in the event of a temperature increase. The additional volume presses against the process membrane of a diaphragm seal. The stiffer a process membrane is, the greater its return force, which counteracts a volume change and acts on the measuring cell together with the process pressure, thus shifting the zero point.

**Pressure transmitter**

The pressure transmitter influences the temperature operating range, the TC zero point and the response time as a result of its volume change. The volume change is the volume that has to be shifted to pass through the complete measuring range.

Pressure transmitters from Endress+Hauser are optimized with regard to minimum volume change.

## Diaphragm seal fill fluid

| Medium               | $P_{abs} = 0.05 \text{ bar (0.725 psi)}^{1)}$ | $P_{abs} \geq 1 \text{ bar (14.5 psi)}^{2)}$       |
|----------------------|-----------------------------------------------|----------------------------------------------------|
| Silicone oil         | -40 to +180 °C (-40 to +356 °F)               | -40 to +250 °C (-40 to +482 °F)                    |
| High-temperature oil | -20 to +200 °C (-4 to +392 °F)                | -20 to +400 °C (-4 to +752 °F) <sup>3) 4) 5)</sup> |
| Low-temperature oil  | -70 to +120 °C (-94 to +248 °F)               | -70 to +180 °C (-94 to +356 °F)                    |
| Vegetable oil        | -10 to +160 °C (+14 to +320 °F)               | -10 to +220 °C (+14 to +428 °F)                    |
| Inert oil            | -40 to +100 °C (-40 to +212 °F)               | -40 to +175 °C (-40 to +347 °F) <sup>6) 7)</sup>   |

- 1) Permitted temperature range at  $p_{abs} = 0.05 \text{ bar (0.725 psi)}$  (observe temperature limits of the device and the system!)
- 2) Permitted temperature range at  $p_{abs} \geq 1 \text{ bar (14.5 psi)}$  (observe temperature limits of the device and the system!)
- 3) 325 °C (617 °F) at  $\geq 1 \text{ bar (14.5 psi)}$  absolute pressure.
- 4) 350 °C (662 °F) at  $\geq 1 \text{ bar (14.5 psi)}$  absolute pressure (max. 200 hours).
- 5) 400 °C (752 °F) at  $\geq 1 \text{ bar (14.5 psi)}$  absolute pressure (max. 10 hours).
- 6) 150 °C (302 °F) at  $\geq 1 \text{ bar (14.5 psi)}$  absolute pressure.
- 7) 175 °C (347 °F) at  $\geq 1 \text{ bar (14.5 psi)}$  absolute pressure (max. 200 hours).

The calculation of the operating temperature range of a diaphragm seal system depends on the fill fluid, capillary length and capillary internal diameter, process temperature and oil volume of the diaphragm seal. Detailed calculations, e.g. for temperature ranges, vacuum pressure and temperature ranges, are done separately in the Applicator ["Sizing Diaphragm Seal"](#).



A0038925

## Information on cleaning

Endress+Hauser provides flushing rings as an accessory to enable cleaning of the process membrane without removing the transmitter from the process.



For further information please contact your local Endress+Hauser Sales Center.

We recommend you perform CIP (cleaning in place (hot water)) before SIP (sterilization in place (steam)) for inline seals. Frequent use of SIP cleaning increases the stress and strain on the process membrane. Under unfavorable conditions, frequent changes of temperature can lead to process membrane material fatigue and potentially leaks over the long term.

## Installation instructions

### Diaphragm seal systems

- A diaphragm seal together with the transmitter form a closed, calibrated system, which has been filled through openings in the diaphragm seal and in the transmitter's measurement system. These openings are sealed and must not be opened.
- For devices with a temperature isolator or capillary, a suitable fastening device (mounting bracket) is recommended.
- When mounting, sufficient strain relief must be provided for the capillary line to prevent the capillary from bending (capillary bending radius  $\geq 100 \text{ mm (3.94 in)}$ )
- For more detailed installation instructions, Endress+Hauser provides its customers with the free "Applicator Sizing Diaphragm Seal" selection tool, which is available online at ["www.endress.com/applicator"](http://www.endress.com/applicator) or as a download.

### Capillary


In order to obtain more precise measurement results and to avoid a defect in the device, mount the capillaries as follows:

- Vibration-free (in order to avoid additional pressure fluctuations)
- Not in the vicinity of heating or cooling lines
- Insulate the capillaries if the ambient temperature is below or above the reference temperature
- With a bending radius  $\geq 100$  mm (3.94 in)
- When using diaphragm seal systems with a capillary, sufficient strain relief must be provided to prevent the capillary from bending (capillary bending radius  $\geq 100$  mm (3.94 in)).
- In the case of devices with capillaries, the zero point shift caused by the hydrostatic pressure of the fill fluid column in the capillaries must be taken into account when selecting the measuring cell. If a measuring cell with a small measuring range is selected, a position adjustment can cause range violation.

### Thermal insulation

#### *Thermal insulation with diaphragm seal directly mounted*


The PMP75 must only be insulated up to a certain height. The maximum permitted insulation height is indicated on the devices and applies to an insulation material with a heat conductivity  $\leq 0.04$  W/(m x K) and to the maximum permitted ambient and process temperature. The data were determined under the most critical application "quiescent air". Maximum permitted insulation height, here indicated on a PMP75 with a flange:

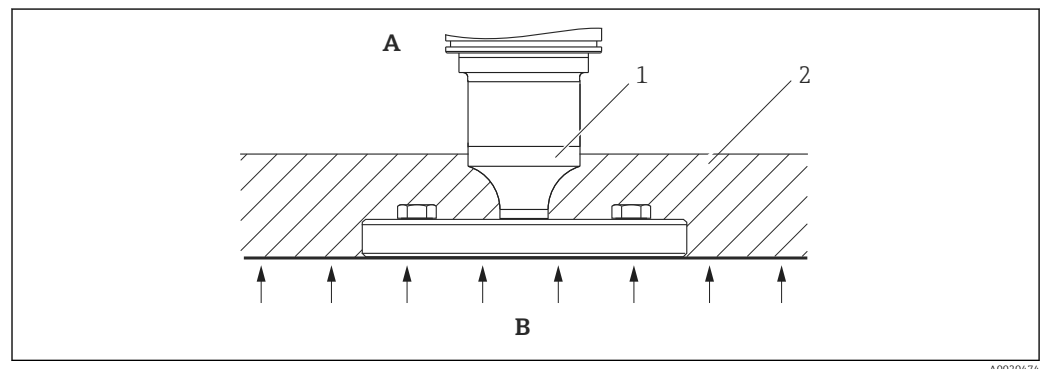

A0020474

- A Ambient temperature  
 B Process temperature  
 1 Maximum permitted insulation height  
 2 Insulation material

Installation with direct mounting

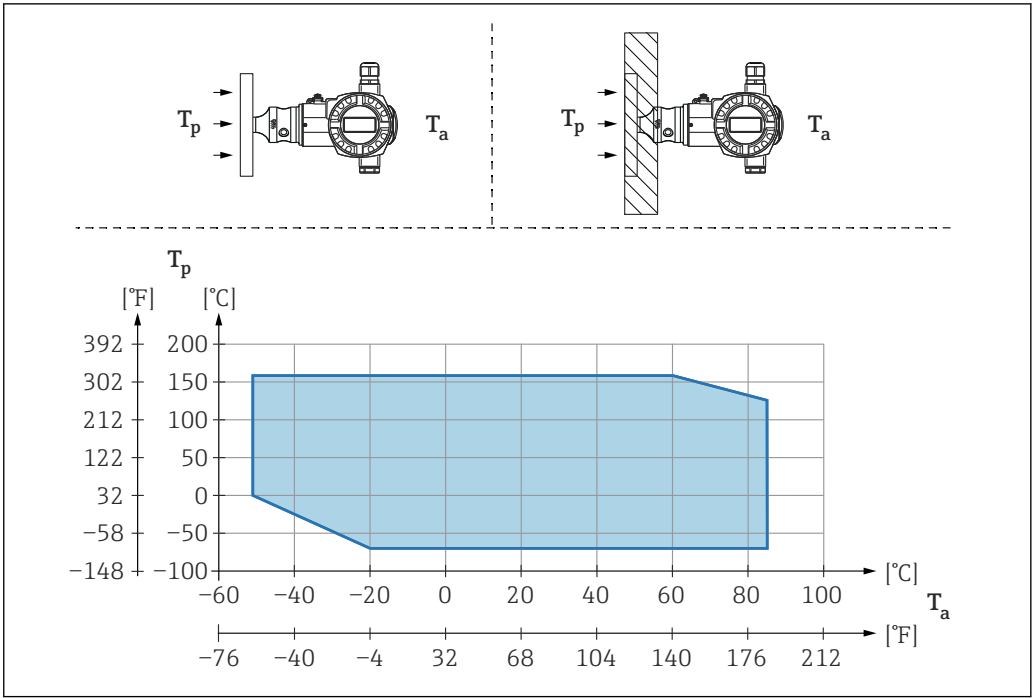

A0043893

$T_a$  Ambient temperature at transmitter

$T_p$  Maximum process temperature


| $T_a$            | $T_p$                           |
|------------------|---------------------------------|
| +85 °C (+185 °F) | -70 to +120 °C (-94 to +248 °F) |
| +60 °C (+140 °F) | -70 to +160 °C (-94 to +320 °F) |
| -20 °C (-4 °F)   | -70 to +160 °C (-94 to +320 °F) |
| -50 °C (-58 °F)  | 0 to +160 °C (+32 to +320 °F)   |

Mounting with temperature isolator

Use of temperature isolators in the event of constant extreme medium temperatures which cause the maximum permissible electronics temperature of +85 °C (+185 °F) to be exceeded. Diaphragm seal systems with temperature isolators can be used up to a maximum temperature of +400 °C (+752 °F) depending on the fill fluid used. . To minimize the influence of rising heat, mount the device horizontally or with the housing pointing downwards. The additional installation height causes a zero point shift of maximum 21 mbar (0.315 psi) due to the hydrostatic column in the temperature isolator. This zero point shift can be corrected on the device.

The maximum ambient temperature  $T_a$  at the transmitter depends on the maximum process temperature  $T_p$ .

The maximum process temperature depends on the diaphragm seal fill fluid used.

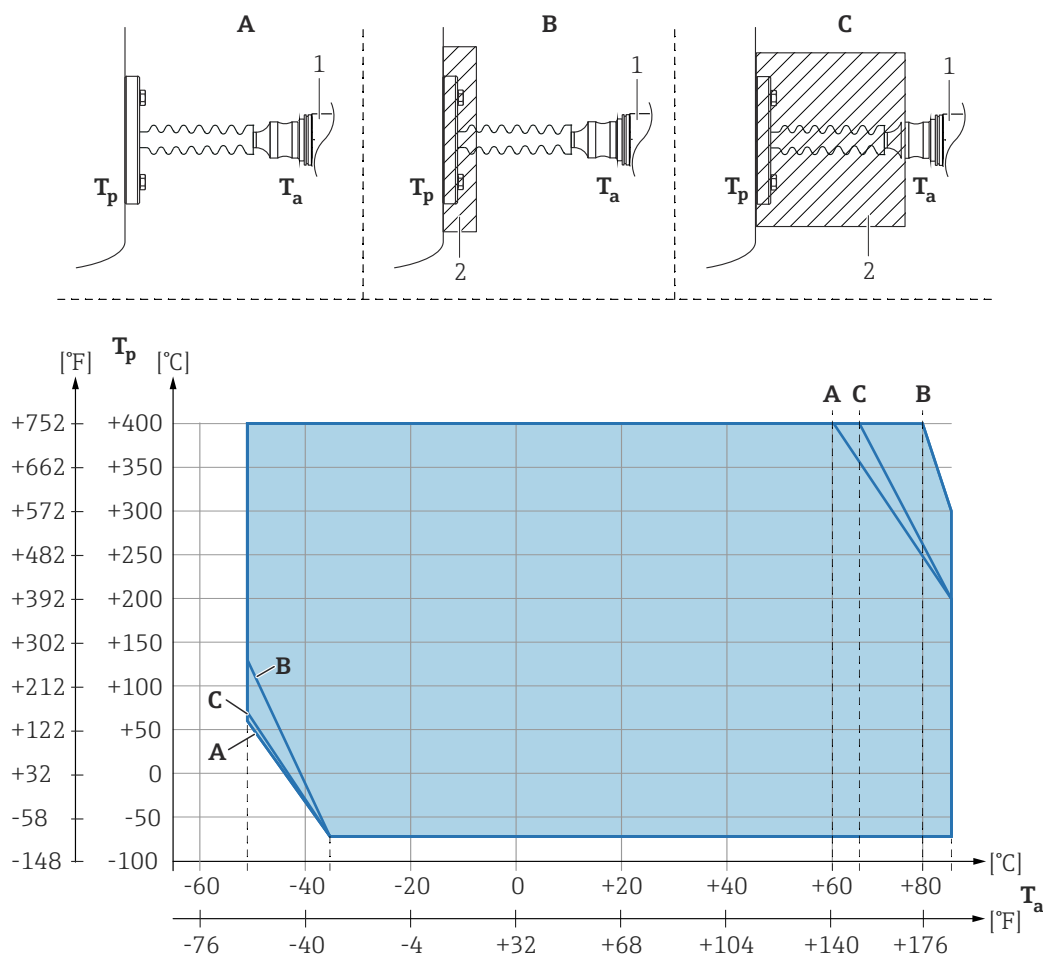

A0039378

- A No insulation  
 B Insulation 30 mm (1.18 in)  
 C Maximum insulation  
 1 Transmitter  
 2 Insulation material

| Item | T <sub>a</sub> <sup>1)</sup> | T <sub>p</sub> <sup>2)</sup>  |
|------|------------------------------|-------------------------------|
| A    | 60 °C (140 °F)               | 400 °C (752 °F) <sup>3)</sup> |
|      | 85 °C (185 °F)               | 200 °C (392 °F)               |
|      | -50 °C (-58 °F)              | 60 °C (140 °F)                |
|      | -35 °C (-31 °F)              | -70 °C (-94 °F)               |
| B    | 80 °C (176 °F)               | 400 °C (752 °F) <sup>3)</sup> |
|      | 85 °C (185 °F)               | 300 °C (572 °F)               |
|      | -50 °C (-58 °F)              | 130 °C (266 °F)               |
|      | -35 °C (-31 °F)              | -70 °C (-94 °F)               |
| C    | 67 °C (153 °F)               | 400 °C (752 °F) <sup>3)</sup> |
|      | 85 °C (185 °F)               | 200 °C (392 °F)               |
|      | -50 °C (-58 °F)              | 70 °C (158 °F)                |
|      | -35 °C (-31 °F)              | -70 °C (-94 °F)               |


- 1) Maximum ambient temperature at transmitter  
 2) Maximum process temperature  
 3) Process temperature: +400 °C (+752 °F) max. depending on the diaphragm seal fill fluid used

**Vacuum applications****Mounting instructions**

For vacuum applications, pressure transmitters with a ceramic process membrane (oil-free) are preferable.


For applications under vacuum, Endress+Hauser recommends mounting the pressure transmitter below the diaphragm seal. This prevents vacuum loading of the diaphragm seal caused by the presence of fill fluid in the capillary.

When the pressure transmitter is mounted above the diaphragm seal, the maximum height difference  $H1$  in accordance with the diagrams below must not be exceeded. The following graphic describes installation above the lower diaphragm seal:

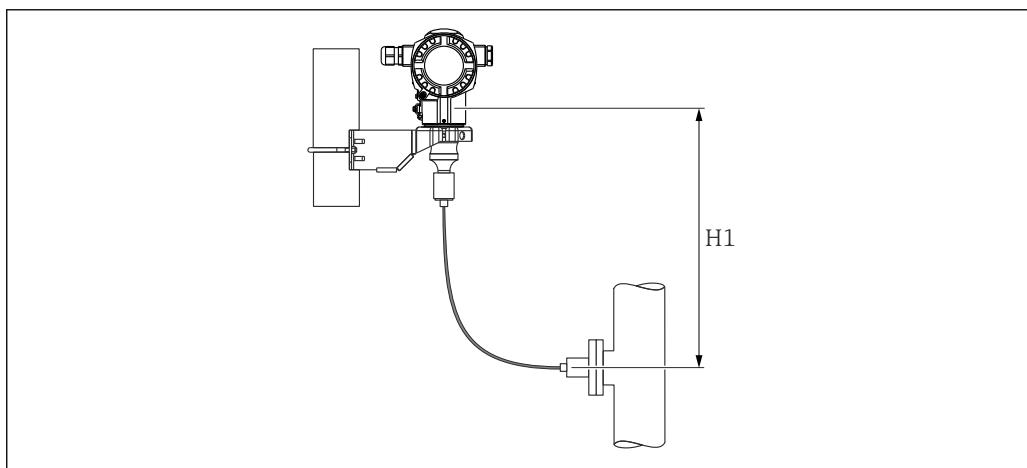

A0020472

The maximum height difference depends on the density of the fill fluid and the smallest ever pressure that is permitted to occur at the diaphragm seal (empty vessel), see the diagram below. The following diagram depicts the maximum installation height above the diaphragm seal for vacuum applications.

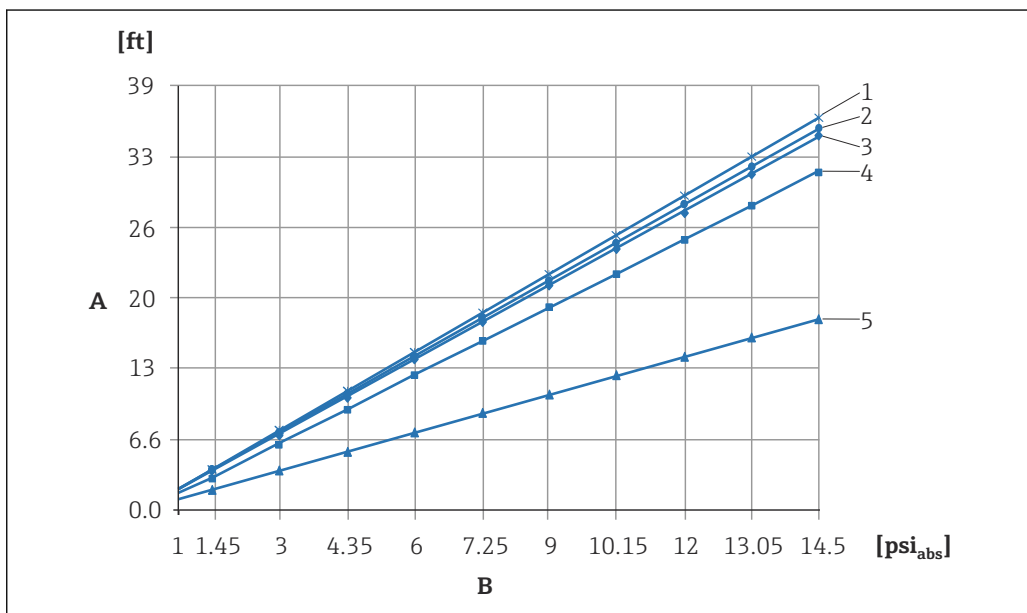

A0023986-EN

- A Height difference  $H1$   
 B Pressure at diaphragm seal  
 1 Low-temperature oil  
 2 Vegetable oil  
 3 Silicone oil  
 4 High-temperature oil  
 5 Inert oil

## Certificates and approvals

Current certificates and approvals for the product are available at [www.endress.com](http://www.endress.com) on the relevant product page:

1. Select the product using the filters and search field.
2. Open the product page.
3. Select **Downloads**.

|                                                                     |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
|---------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| <b>CE mark</b>                                                      | The device meets the legal requirements of the relevant EC directives. Endress+Hauser confirms that the device has been successfully tested by applying the CE mark.                                                                                                                                                                                                                                                                                                                                                                                                                |
| <b>RoHS</b>                                                         | The measuring system complies with European Directive 2002/96/EC.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   |
| <b>RCM-Tick marking</b>                                             | <p>The supplied product or measuring system meets the ACMA (Australian Communications and Media Authority) requirements for network integrity, interoperability, performance characteristics as well as health and safety regulations. Here, especially the regulatory arrangements for electromagnetic compatibility are met. The products bear the RCM-Tick marking on the nameplate.</p> <div style="text-align: center;">  </div> <p style="text-align: right; font-size: small;">A0029561</p> |
| <b>TSE (BSE) compliance (ADI free - Animal Derived Ingredients)</b> | <p>As the manufacturer, Endress+Hauser states:</p> <ul style="list-style-type: none"> <li>■ That the parts of this product in contact with the process are not made from materials derived from animals <b>or</b></li> <li>■ at least comply with the requirements of guidelines outlined in EMA/410/01 rev. 3 (TSE (BSE) compliance).</li> </ul>                                                                                                                                                                                                                                   |
| <b>Ex approvals</b>                                                 | <ul style="list-style-type: none"> <li>■ ATEX</li> <li>■ FM</li> <li>■ CSA</li> <li>■ NEPSI</li> <li>■ IECEx</li> <li>■ TIIS</li> <li>■ Also combinations of different approvals</li> </ul> <p>All explosion protection data are given in separate documentation which is available upon request. The Ex documentation is supplied as standard with all Ex-systems .</p>                                                                                                                                                                                                            |
| <b>Corrosion test</b>                                               | <p>Standards and test methods:</p> <ul style="list-style-type: none"> <li>■ 316L: ASTM A262 Practice E and ISO 3651-2 Method A</li> <li>■ Alloy C22 and Alloy C276: ASTM G28 Practice A and ISO 3651-2 Method C</li> <li>■ 22Cr duplex, 25Cr duplex: ASTM G48 Practice A or ISO 17781 and ISO 3651-2 Method C</li> </ul> <p>The corrosion test is confirmed for all wetted and pressure-bearing parts.</p> <p>A 3.1 material certificate must be ordered as confirmation of the test.</p>                                                                                           |
| <b>EAC conformity</b>                                               | <p>The measuring system meets the legal requirements of the applicable EAC guidelines. These are listed in the corresponding EAC Declaration of Conformity along with the standards applied.</p> <p>Endress+Hauser confirms successful testing of the device by affixing to it the EAC mark.</p>                                                                                                                                                                                                                                                                                    |
| <b>Suitable for hygiene applications</b>                            | <p>For information on installation and approvals, see documentation SD02503F "Hygiene approvals".</p> <p>For information on 3-A and EHEDG-tested adapters, see documentation TI00426F "Weld-in adapter, process adapter and flanges".</p>                                                                                                                                                                                                                                                                                                                                           |
| <b>Certificate of current Good Manufacturing Practices (cGMP)</b>   | Product Configurator, order code for "Test, Certificate" option "JG"                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |

- The certificate is only available in English
- Materials of construction of product wetted parts
- TSE compliance
- Polishing and surface finish
- Material/ compound compliance table (USP Class VI, FDA conformity)

#### Functional safety SIL/ IEC 61508 Declaration of Conformity (optional)

The Cerabar S with 4 to 20 mA output signal has been developed in accordance with the IEC 61508 standard. These devices can be used to monitor the process level and pressure up to SIL 3. For a detailed description of safety functions with the Cerabar S, settings and functional safety data, see the "Functional safety manual - Cerabar S" SD00190P/00.

For devices up to SIL 3 / IEC 61508 Declarations of Conformity see:

Ordering information:

Product Configurator, order code for "Additional options 1" and "Additional options 2", version "E".

#### CRN approval

- PMC71: Some device versions have CRN approval. These devices are fitted with a separate plate bearing the registration number CRN OF23358.5C.
- PMP71: Some device versions have CRN approval. These devices are fitted with a separate plate bearing the registration number CRN OF22502.5C.
- PMP75 devices with a capillary are not CRN-approved.

A CRN-approved process connection can be obtained in one of the following ways:

- CRN-approved process connection must be ordered with a CSA approval
- CRN-approved process connection must be ordered with the "CRN" option in the order code for "Additional approval"

#### Pressure Equipment Directive 2014/68/EU (PED)

##### Pressure equipment with permitted pressure $\leq 200$ bar (2 900 psi)

Pressure equipment (maximum allowable pressure (MWP)  $PS \leq 200$  bar (2 900 psi)) can be classified as pressure accessories in accordance with Pressure Equipment Directive 2014/68/EU. If the maximum allowable pressure is  $\leq 200$  bar (2 900 psi) and the pressurized volume of the pressure equipment is  $\leq 0.1$  l, the pressure equipment is subject to the Pressure Equipment Directive (see Pressure Equipment Directive 2014/68/EU, Article 4, point 3). The Pressure Equipment Directive only requires that the pressure equipment shall be designed and manufactured in accordance with the "sound engineering practice of a Member State".

Reasons:

- Pressure Equipment Directive (PED) 2014/68/EU Article 4, point 3
- Pressure Equipment Directive 2014/68/EU, Commission's Working Group "Pressure", Guideline A-05 + A-06

Note:

A partial examination shall be performed for pressure instruments that are part of safety equipment for the protection of a pipe or vessel from exceeding allowable limits (safety accessory in accordance with Pressure Equipment Directive 2014/68/EU Article 2, point 4).

##### Pressure equipment with allowable pressure $> 200$ bar (2 900 psi)

Pressure equipment designated for application in every process fluid having a pressurized volume of  $< 0.1$  l and a maximum allowable pressure  $PS > 200$  bar (2 900 psi) shall satisfy the essential safety requirements set out in Annex I of the Pressure Equipment Directive 2014/68/EU. According to Article 13, pressure equipment shall be classified by categories in accordance with Annex II. Taking into account the low volume specified above, the pressure instruments can be categorized as category I pressure equipment. They must then bear a CE mark.

Reasons:

- Pressure Equipment Directive 2014/68/EU, Article 13, Annex II
- Pressure Equipment Directive 2014/68/EU, Commission's Working Group "Pressure", Guideline A-05

Note:

A partial examination shall be performed for pressure instruments that are part of safety equipment for the protection of a pipe or vessel from exceeding allowable limits (safety accessory in accordance with Pressure Equipment Directive 2014/68/EU, Article 2, point 4).

The following also applies:

- PMP71 with thread and internal process membrane PN > 200 and oval flange adapter PN > 200:  
Suitable for stable gases in group 1, category I, module A
- PMP75 with inline seal  $\geq 1.5"/\text{PN}40$ :  
Suitable for stable gases in group 1, category II, module A2
- PMP75 with separators PN > 200  $\geq 1.5"/\text{PN}40$ :  
Suitable for stable gases in group 1, category I, module A
- PMP75 with thread PN > 200:  
Suitable for stable gases in group 1, category I, module A

#### MID Parts Certificate

TC7975

#### Classification of process sealing between electrical systems and (flammable or combustible) process fluids in accordance with ANSI/ISA 12.27.01

Endress+Hauser devices are designed in accordance with ANSI/ISA 12.27.01, allowing the user to waive the use of - and save the cost of installing - external secondary process seals in the conduit as required by the process sealing sections of ANSI/NFPA 70 (NEC) and CSA 22.1 (CEC). These instruments comply with the North-American installation practice and provide a very safe and cost-saving installation for pressurized applications with hazardous fluids. Please refer to the following table for the seal class assigned (single seal or dual seal):

| Device | Approval           | Remark                | Single seal MWP                         | Dual seal MWP              |
|--------|--------------------|-----------------------|-----------------------------------------|----------------------------|
| PMC71  | CSA C/US IS, XP    | W/o separate housing  | -                                       | 60 bar (900 psi)           |
|        | CSA C/US IS        | With separate housing | 40 bar (600 psi)                        | -                          |
| PMP71  | CSA C/US XP, XP+IS | W/o separate housing  | 400 bar (6 000 psi)                     | -                          |
|        | CSA C/US IS        | W/o separate housing  | >200 to 400 bar<br>(3 000 to 6 000 psi) | $\leq 200$ bar (3 000 psi) |
|        | CSA C/US IS        | With separate housing | 400 bar (6 000 psi)                     | -                          |
| PMP75  | XP, XP+IS          | W/o separate housing  | 400 bar (6 000 psi)                     | -                          |
|        | CSA C/US IS        | W/o separate housing  | >200 to 400 bar<br>(3 000 to 6 000 psi) | $\leq 200$ bar (3 000 psi) |
|        | CSA C/US IS        | With separate housing | 400 bar (6 000 psi)                     | -                          |

Further information can be found in the control drawings of the relevant devices.

#### Inspection certificate

| Designation                                                                                             | PMC71 | PMP71 | PMP75 | Option              |
|---------------------------------------------------------------------------------------------------------|-------|-------|-------|---------------------|
| 3.1 Material documentation, wetted metal parts, EN10204-3.1 inspection certificate                      | ✓     | ✓     | ✓     | B <sup>1) 3)</sup>  |
| Declaration of Conformity NACE MR0175, wetted metal parts                                               | —     | ✓     | ✓     | C <sup>1) 3)</sup>  |
| EN10204-3.1 material, NACE MR0175, wetted metal parts, inspection certificate                           | —     | ✓     | ✓     | D <sup>1) 3)</sup>  |
| Individual test, test report                                                                            | ✓     | ✓     | ✓     | 3 <sup>1)</sup>     |
| Pressure test, internal procedure, test report                                                          | ✓     | ✓     | ✓     | 4 <sup>1)</sup>     |
| Helium leak test, internal procedure, test report                                                       | ✓     | ✓     | —     | 5 <sup>1)</sup>     |
| EN10204-3.1 material wetted parts +Ra, Ra= surface roughness, dimensional check, inspection certificate | ✓     | —     | —     | 6 <sup>1)</sup>     |
| Delta ferrite measurement, internal procedure, wetted metal parts, inspection certificate               | ✓     | —     | —     | 8 <sup>1)</sup>     |
| 3.1 Material documentation, wetted metal parts, EN10204-3.1 inspection certificate                      | ✓     | ✓     | ✓     | JA <sup>2) 3)</sup> |
| Declaration of Conformity NACE MR0175, wetted metal parts                                               | ✓     | ✓     | ✓     | JB <sup>2) 3)</sup> |
| Declaration of Conformity NACE MR0103, wetted metal parts                                               | ✓     | ✓     | ✓     | JE <sup>2) 3)</sup> |
| Surface finish measurement ISO4287/Ra, wetted metal parts, inspection certificate                       | ✓     | —     | ✓     | KB <sup>2)</sup>    |
| Helium leak test, internal procedure, inspection certificate                                            | ✓     | ✓     | ✓     | KD <sup>2)</sup>    |
| Pressure test, internal procedure, inspection certificate                                               | ✓     | ✓     | ✓     | KE <sup>2)</sup>    |

| Designation                                                                               | PMC71 | PMP71 | PMP75 | Option           |
|-------------------------------------------------------------------------------------------|-------|-------|-------|------------------|
| Delta ferrite measurement, internal procedure, wetted metal parts, inspection certificate | ✓     | —     | ✓     | KF <sup>2)</sup> |
| PMI test (XRF), internal procedure, metal parts in contact with the medium                | ✓     | ✓     | ✓     | KG <sup>2)</sup> |
| Welding documentation, wetted/pressurized seams                                           | —     | ✓     | —     | KS <sup>2)</sup> |

- 1) Product Configurator, order code for "Additional options 1" and "Additional options 2"
- 2) Product Configurator, order code for "Test, Certificate"
- 3) The choice of this feature for coated process membranes/process connections refers to the metal base material.

## Ordering information

Detailed ordering information is available from the following sources:

- In the Product Configurator on the Endress+Hauser website: [www.endress.com](http://www.endress.com) -> Click "Corporate" -> Select your country -> Click "Products" -> Select the product using the filters and search field -> Open product page -> The "Configure" button to the right of the product image opens the Product Configurator.
- From your Endress+Hauser Sales Center: [www.addresses.endress.com](http://www.addresses.endress.com)



### Product Configurator - the tool for individual product configuration

- Up-to-the-minute configuration data
  - Depending on the device: Direct input of measuring point-specific information such as measuring range or operating language
  - Automatic verification of exclusion criteria
  - Automatic creation of the order code and its breakdown in PDF or Excel output format
  - Ability to order directly in the Endress+Hauser Online Shop

#### Special device versions

Endress+Hauser offers special device versions as **Technical Special Products (TSP)**.

For further information please contact your local Endress+Hauser Sales Center.

#### Scope of delivery

- Measuring device
- Optional accessories
- Brief Operating Instructions
- Calibration certificates
- Optional certificates

#### Measuring point (TAG)

|                                               |                                                                                                                                                                                                                                                                                                                                                                    |
|-----------------------------------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Order code                                    | 895: Marking                                                                                                                                                                                                                                                                                                                                                       |
| Option                                        | Z1: Tagging (TAG), see additional spec.                                                                                                                                                                                                                                                                                                                            |
| Position of the measuring point marking       | To be selected in the additional specifications: <ul style="list-style-type: none"> <li>■ Tag plate Stainless Steel</li> <li>■ Self-adhesive paper label</li> <li>■ Supplied label/plate</li> <li>■ RFID TAG</li> <li>■ RFID TAG + Tag plate Stainless Steel</li> <li>■ RFID TAG + Self-adhesive paper label</li> <li>■ RFID TAG + Supplied label/plate</li> </ul> |
| Definition of the measuring point designation | To be defined in the additional specifications:<br>3 lines containing up to 18 characters each<br>The measuring point designation appears on the selected label and/or the RFID TAG.                                                                                                                                                                               |
| Identification on electronic nameplate (ENP)  | 32 characters                                                                                                                                                                                                                                                                                                                                                      |

Configuration data sheet

Pressure

The following configuration data sheet must be completed and included with the order if the option "E" or "H" has been selected in the Product Configurator, order code for "Calibration; Unit".

| Pressure unit                 |                                                           |                                              |                                 |                                             |
|-------------------------------|-----------------------------------------------------------|----------------------------------------------|---------------------------------|---------------------------------------------|
| <input type="checkbox"/> mbar | <input type="checkbox"/> mmH <sub>2</sub> O <sup>1)</sup> | <input type="checkbox"/> mmHg <sup>2)</sup>  | <input type="checkbox"/> Pascal | <input type="checkbox"/> torr               |
| <input type="checkbox"/> bar  | <input type="checkbox"/> mH <sub>2</sub> O <sup>1)</sup>  | <input type="checkbox"/> inHg <sup>2)</sup>  | <input type="checkbox"/> hPa    | <input type="checkbox"/> g/cm <sup>2</sup>  |
| <input type="checkbox"/> psi  | <input type="checkbox"/> ftH <sub>2</sub> O <sup>1)</sup> | <input type="checkbox"/> gf/cm <sup>2</sup>  | <input type="checkbox"/> kPa    | <input type="checkbox"/> kg/cm <sup>2</sup> |
|                               | <input type="checkbox"/> inH <sub>2</sub> O <sup>1)</sup> | <input type="checkbox"/> kgf/cm <sup>2</sup> | <input type="checkbox"/> MPa    | <input type="checkbox"/> lb/ft <sup>2</sup> |
|                               |                                                           |                                              |                                 | <input type="checkbox"/> atm                |

- 1) The conversion factor for the pressure unit is based on a reference temperature of 4 °C (39.2 °F).  
2) The conversion factor of the pressure unit refers to a reference temperature of 0 °C (32 °F).

| Calibration Range / Output |                                   |
|----------------------------|-----------------------------------|
| Low range value (LRV):     | _____ [Pressure engineering unit] |
| Upper range value (URV):   | _____ [Pressure engineering unit] |

| Display                                                                                      |
|----------------------------------------------------------------------------------------------|
| Display of the content of the main line (option depends on sensor and communication variant) |
| <input type="checkbox"/> Primary value [PV] (default)                                        |
| <input type="checkbox"/> Main Value [%]                                                      |
| <input type="checkbox"/> Pressure                                                            |
| <input type="checkbox"/> Current [mA] (HART only)                                            |
| <input type="checkbox"/> Temperature                                                         |
| <input type="checkbox"/> Error number                                                        |
| <input type="checkbox"/> Alternating display                                                 |


| Damping                            |
|------------------------------------|
| Damping: _____ sec (Default 2 sec) |

Smallest calibratable span (preset at factory) → 11

The following configuration data sheet must be completed and included with the order if the option "F" or "T" has been selected in the Product Configurator, order code for "Calibration; Unit".

| Pressure unit                                                                                 |                                                                                                                                                                                                                                                 |                                                                                                                                                                                           |                                                                                                                                 |                                                                                                                                                                                                           | Output unit (scaled unit)                                                                        |                                                                                                                                                                                                    |                                                                                                                                                            |                                                                                                                       |                                       |
|-----------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------|---------------------------------------|
| <input type="checkbox"/> mbar<br><input type="checkbox"/> bar<br><input type="checkbox"/> psi | <input type="checkbox"/> mmH <sub>2</sub> O <sup>1)</sup><br><input type="checkbox"/> mH <sub>2</sub> O <sup>1)</sup><br><input type="checkbox"/> ftH <sub>2</sub> O <sup>1)</sup><br><input type="checkbox"/> inH <sub>2</sub> O <sup>1)</sup> | <input type="checkbox"/> mmHg <sup>2)</sup><br><input type="checkbox"/> inHg <sup>2)</sup><br><input type="checkbox"/> gf/cm <sup>2</sup><br><input type="checkbox"/> kgf/cm <sup>2</sup> | <input type="checkbox"/> Pascal<br><input type="checkbox"/> hPa<br><input type="checkbox"/> kPa<br><input type="checkbox"/> MPa | <input type="checkbox"/> torr<br><input type="checkbox"/> g/cm <sup>2</sup><br><input type="checkbox"/> kg/cm <sup>2</sup><br><input type="checkbox"/> lb/ft <sup>2</sup><br><input type="checkbox"/> atm | Mass<br><input type="checkbox"/> kg<br><input type="checkbox"/> t<br><input type="checkbox"/> lb | Lengths<br><input type="checkbox"/> m<br><input type="checkbox"/> dm<br><input type="checkbox"/> cm<br><input type="checkbox"/> mm<br><input type="checkbox"/> ft<br><input type="checkbox"/> inch | Volume<br><input type="checkbox"/> l<br><input type="checkbox"/> hl<br><input type="checkbox"/> m <sup>3</sup><br><input type="checkbox"/> ft <sup>3</sup> | Volume<br><input type="checkbox"/> USgal<br><input type="checkbox"/> impgal<br><input type="checkbox"/> USbblPE<br>TR | Percent<br><input type="checkbox"/> % |
| Empty calibration [a]:<br>Low pressure value (empty)                                          |                                                                                                                                                                                                                                                 |                                                                                                                                                                                           |                                                                                                                                 |                                                                                                                                                                                                           | Empty calibration [a]:<br>Low level value (empty)                                                |                                                                                                                                                                                                    |                                                                                                                                                            |                                                                                                                       |                                       |
| <input type="text"/><br>[Pressure engineering unit]                                           |                                                                                                                                                                                                                                                 |                                                                                                                                                                                           |                                                                                                                                 |                                                                                                                                                                                                           | <input type="text"/><br>[Scaled Unit]                                                            |                                                                                                                                                                                                    |                                                                                                                                                            |                                                                                                                       |                                       |
| Full calibration [b]:<br>High pressure value (full)                                           |                                                                                                                                                                                                                                                 |                                                                                                                                                                                           |                                                                                                                                 |                                                                                                                                                                                                           | Full calibration [b]:<br>High level value (full)                                                 |                                                                                                                                                                                                    |                                                                                                                                                            |                                                                                                                       |                                       |
| <input type="text"/><br>[Pressure engineering unit]                                           |                                                                                                                                                                                                                                                 |                                                                                                                                                                                           |                                                                                                                                 |                                                                                                                                                                                                           | <input type="text"/><br>[Scaled Unit]                                                            |                                                                                                                                                                                                    |                                                                                                                                                            |                                                                                                                       |                                       |

**Example**

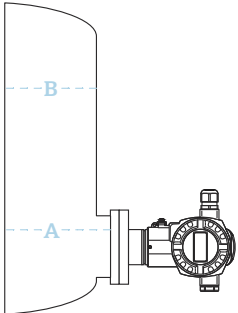

A    0 mbar / 0m

B    300 mbar (4.5 psi) / 3 m (9.8 ft)

A0020477

- 1) The conversion factor for the pressure unit is based on a reference temperature of 4 °C (39.2 °F).
- 2) The conversion factor of the pressure unit refers to a reference temperature of 0 °C (32 °F).

| Display                                                                                      |                              |
|----------------------------------------------------------------------------------------------|------------------------------|
| Display of the content of the main line (option depends on sensor and communication variant) |                              |
| <input type="checkbox"/>                                                                     | Primary value [PV] (default) |
| <input type="checkbox"/>                                                                     | Main Value [%]               |
| <input type="checkbox"/>                                                                     | Pressure                     |
| <input type="checkbox"/>                                                                     | Current [mA] (HART only)     |
| <input type="checkbox"/>                                                                     | Temperature                  |
| <input type="checkbox"/>                                                                     | Level before Lin.            |
| <input type="checkbox"/>                                                                     | Tank content                 |
| <input type="checkbox"/>                                                                     | Error number                 |
| <input type="checkbox"/>                                                                     | Alternating display          |

## Accessories

|                                      |                                                                                                                                                                                                                                                                                                         |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
|--------------------------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| HistoROM®/M-DAT                      | The HistoROM®/M-DAT is a memory module that can be attached to any electronic insert (not for 1-5V DC).<br><br>Ordering information:<br><br>Product Configurator, order code for "Additional options 1" or Additional options 2", version "N" or as a separate accessory (part no.: 52027785).          |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| Welding flanges and weld-in adapters | For details, refer to TI00426F/00/EN "Weld-in adapters, process adapters and flanges".                                                                                                                                                                                                                  |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| Manifolds                            | See the →  76.<br><br>For further details, see SD01553P/00/EN "Mechanical accessories for pressure measuring devices".                                                                                                 |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| Additional mechanical accessories    | Oval flange adapters, pressure gauge valves, shutoff valves, siphons, condensate pots, cable shortening kits, test adapters, mounting brackets, flushing rings, block&bleed valves and protective roofs.<br><br>For details see SD01553P/00/EN "Mechanical accessories for pressure measuring devices". |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
| Service-specific accessories         |                                                                                                                                                                                                                                                                                                         |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       |
|                                      | Accessories                                                                                                                                                                                                                                                                                             | Description                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
|                                      | DeviceCare SFE100                                                                                                                                                                                                                                                                                       | Configuration tool for HART, PROFIBUS and FOUNDATION Fieldbus field devices<br> Technical Information TI01134S<br><br> DeviceCare is available for download at <a href="http://www.software-products.endress.com">www.software-products.endress.com</a> . You need to register in the Endress+Hauser software portal to download the application.                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |
|                                      | FieldCare SFE500                                                                                                                                                                                                                                                                                        | FDT-based plant asset management tool<br>FieldCare can configure all smart field units in your plant and helps you manage them. By using the status information, FieldCare is also a simple but effective way of checking the status and condition of the field devices.<br><br> Technical Information TI00028S                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |
|                                      | Field Xpert SMT70, SMT77                                                                                                                                                                                                                                                                                | The Field Xpert SMT70 tablet PC for device configuration enables mobile plant asset management in hazardous (Ex Zone 2) and non-hazardous areas. It is suitable for commissioning and maintenance staff. It manages Endress+Hauser and third-party field instruments with a digital communication interface and documents the progress of the work. The SMT70 is designed as a complete solution. It comes with a pre-installed driver library and is an easy-to-use, touch-enabled tool for managing field devices throughout their entire life cycle.<br>The Field Xpert SMT77 for device configuration enables mobile plant asset management in areas categorized as Ex Zone 1. It is suitable for commissioning and maintenance staff for easy management of field instruments with a digital communication interface. The touch-enabled tablet PC is designed as a complete solution. It comes with comprehensive pre-installed driver libraries and offers users a modern software user interface to manage field instruments throughout the entire life cycle. |

## Documentation



For an overview of the scope of the associated Technical Documentation, refer to the following:

- *Device Viewer* ([www.endress.com/deviceviewer](http://www.endress.com/deviceviewer)): Enter the serial number from the nameplate
- *Endress+Hauser Operations app*: Enter serial number from nameplate or scan matrix code on nameplate.

---

### Standard documentation

#### Document type: Operating Instructions (BA)

Installation and initial commissioning – contains all the functions in the operating menu that are needed for a routine measuring task. Functions beyond this scope are not included.

#### Document type: Brief Operating Instructions (KA)

Quick guide to the first measured value – includes all essential information from incoming acceptance to electrical connection.

#### Document type: Safety Instructions, certificates

Depending on the approval, safety instructions are supplied with the device, e.g. XA. This documentation is an integral part of the Operating Instructions. Information on the Safety Instructions (XA) that are relevant for the device is provided on the nameplate.

---

### Supplementary device-dependent documentation

Additional documents are supplied depending on the device version ordered: Always comply strictly with the instructions in the supplementary documentation. The supplementary documentation is an integral part of the device documentation.



71651077

[www.addresses.endress.com](http://www.addresses.endress.com)

---